

37/150

**LIAQUAT UNIVERSITY HOSPITAL
HYDERABAD / JAMSHORO**

**BID
EVALUATION REPORT**

**PURCHASE OF MACHINERY /EQUIPMENT UNDER
SNE/ ADP FOR THE YEAR 2017-18
(RESCUE CENTRE) NEURO- SURGERY
DEPARTMENT (PART-II)
AT LUH, HYDERABAD)**

TENDER NO. 41/2017-18

OPENED ON 27.03.2018 12:00PM




**LIAQUAT UNIVERSITY HOSPITAL
HYDERABAD / JAMSHORO**

**BID
EVALUATION REPORT**

**PURCHASE OF MACHINERY /EQUIPMENT UNDER
SNE/ ADP FOR THE YEAR 2017-18
(RESCUE CENTRE) NEURO- SURGERY
DEPARTMENT (PART-II)
AT LUH, HYDERABAD)**

TENDER NO. 41/2017-18

OPENED ON 27.03.2018 12:00PM



SINDH PUBLIC PROCUREMENT REGULATORY AUTHORITY GOVERNMENT OF SINDH

HOME SPPRA PUBLIC PROCUREMENT NEWS SEND QUERY SPP ACT 2009 SPP RULES NOTIFICATIONS TRAININGS POLICY LETTERS
Search Tenders List

Tenders Notice
S
A Y
BER Date A Y

Serial No. ▲ ▼	SPPRA ID ▲ ▼	Department ▲ ▼	Advertisement Date ▲ ▼	Closing Date ▲ ▼	Upload Date ▲ ▼	City ▲ ▼	BER Date ▲ ▼
37150		liaquat university					
Records per page	50 ▼	Columns	CSV Export	Excel Export	Filter		
37150	2147483647	Liaquat University Hospital	2018-03-05 00:00:00	2018-03-27 23:59:59	06-03-2018	HYDERABAD/JAMSHO RO	

LIAQUAT UNIVERSITY HOSPITAL, HYDERABAD / JAMSHORO
FINANCIAL YEAR 2017-18


S No.	Description of Procurement	Qty	Estimated Total cost	Funds Allocated	Source of funds (ADP / Non ADP)	Proposed Procurement method	Timing of Procurement				Remarks
							1st Qtr	2nd Qtr	3rd Qtr	4th Qtr	
1	Drugs / Medicines & Surgical Items (L.P)		87.75 M	87.75 M	Non ADP	Single Stage Two Envelope	In all quarters as per Requirement				
2	Dietary Items.		40.95 M	40.95 M	---do---	---do---					
3	Uniform & Liveries		3.33 M	3.33 M	---do---	---do---					
4	Misc / Patty / Electric Items.		4.389 M	4.389 M	---do---	---do---					
5	Medical Gases		29.23 M	29.23 M	---do---	---do---					
6	Janitorial Services & Items.		9.45 M	9.45 M	---do---	---do---					
7	Printing Articles.		1.016 M	1.016 M	---do---	---do---					
8	Stationary Articles		0.604 M	0.604 M	---do---	---do---					
9	Instruments		35.464 M	35.464 M	---do---	---do---					
10	Consumable Items / Pathology Kits & Chemicals.		12.183 M	12.183 M	---do---	---do---					
11	Deployment of Security Guards		13.2 M	13.2 M							
12	Repair of Machinery / Equipment		37.077 M	37.077 M	---do---	---do---					
13	Repair of Furniture / Fixture.		2.04 M	2.04 M	---do---	---do---					
14	Drugs/Medicine under Zakat fund (Bulk)		42.0 M	42.0 M	---do---	---do---					
15	Drugs/Medicine under Zakat fund (LP)		28.0 M		---do---	---do---					
16	Repair of Transport		4.692 M	4.692 M	---do---	---do---					
17	Machinery Equipment under SNE		374.14 M	374.14 M	---do---	---do---					
I	Purchase of C.T Scan Machine		70.0 M		---do---	---do---					
II	Purchase of Dialysis Machine		6.00 M		---do---	---do---					
III	Purchase of Lithotripsy Machine		70.0 M		---do---	---do---					
IV	Purchase of M.R.I Machine		125.0 M	374.14 M	---do---	---do---					
V	Purchase of Laundry Machine		4.00 M		---do---	---do---					
18	Purchase of Machiner / Equipment for Paeds		99.140 M		---do---	---do---					
19	Purchase of Machinery from Welfare fund		5.00 M	5.00 M	---do---	---do---					
20	Furniture / Fixture under SNE		58.925 M	58.925 M	---do---	---do---					
21	Purchase of Transport		39.0 M	39.0 M	---do---	---do---					
22	Purchase of Machinery /Equipment under various ADP/Non ADP Scheme & Rescue Center.		400.00 M		ADP	---do---					

List Enclosed



NOTIFICATION

NO.HD (P&E) 1-2 (61) / 2017. In supersession of this department's notification No.HD (P&E) 3-5 (77) / 2017, dated 16.03.2017, NO.HD (P&E) 3-5 (74) / 2013, dated 03.08.2017, NO.HD (P&E) 3-5 (85) / 2017, dated 03.08.2017, NO.HD (P&E) 3-5 (78) / 2013, dated 11.09.2017, NO.HD (P&E) 3-5 (55) / 2015, dated 11.09.2017 and SO (PM&I) 2-1 / 2017-18 / PM-05 (LUH), dated 07.08.2017, the Government of Sindh, Health Department is pleased to re constitute a Procurement Committee under Clause-7 of Sindh Public Procurement Rules 2010 (Amended 2017), comprising of the following members for purchase of machinery / equipment, vehicles and furniture / fixture to be purchased under revenue component of "ADP schemes & SNE" in respect of Liaquat University Hospital Hyderabad;

- | | | |
|---|----------|---|
| 1. Additional Medical Superintendent (General),
Liaquat University Hospital, Hyderabad. | Chairman |  |
| 2. Additional Medical Superintendent (Technical)
Liaquat University Hospital, Hyderabad. | Member | |
| 3. Professor / Associate Professor / Assistant
Professor / Expert / Technical Person of Relevant field,
Liaquat University of Medical & Health Sciences (LUM&HS)
Jamshoro. | Member | |

The committee will responsible to observe all the codal formalities as per Sindh Public Procurement Rules 2010 (Amended 2017), the TORS / Functions / Responsibilities of procurement committee in accordance with SPP Rule-8 (Amended 2017) are as under;

- Preparing bidding documents;
- Carrying out technical as well as financial evaluation of the bids
- Preparing evaluation report as provided in rule-45,
- Making recommendations for the award of contract to the competent authority;
- Perform any other function ancillary and incidental to the above.

(DR.FAZLULLAH PECHUHO)
SECRETARY HEALTH


NO.HD (P&E) 1-2 (61) / 2017


Karachi, dated 07-11-2017.


C.c.to:

- The Vice Chancellor, Liaquat University of Medical and Health Sciences Hyderabad / Jamshoro with request to advice the member to attend the meetings for above said committee.
- The Managing Director, Sindh Public Procurement Regularity Authority, Karachi.
- The Medical Superintendent, Liaquat University Hospital Hyderabad / Jamshoro.
- The District Accounts Officer, Hyderabad.
- All members of the committee.
- P.S. to Secretary, Health Department, Govt. of Sindh, Karachi.
- P.S to Additional Secretary (Dev), Health Department, Govt. of Sindh, Karachi.


Deputy(Director (Dev)









NO.HD(P&E) 3-2 (427)/2014
GOVERNMENT OF SINDH
HEALTH DEPARTMENT
(Procurement, Monitoring and Inspection Cell)
Karachi dated the 10th APRIL, 2017.

NOTIFICATION

No.HD(P&E)3-2(427)/2014. In supersession to this department's notification of even number dated 9-03-2017 and in pursuance of Rule 31 of the Sindh Public Procurement Rules, 2010, a Departmental Complaint Redressal Committee, comprising of following officers is hereby re-constituted as under to resolve complaints of aggrieved bidders:

1. Special Secretary,
Health Department. *19/4 25-4-17* Chairman
2. Representative from Accountant General Sindh, Member
3. Independent expert from relevant field concerning
(to be nominated by the Head of Procuring Agency) Member
4. Deputy Secretary (PM&I) Member
5. Deputy Secretary (General) Member/Secretary

ToRs.

- To perform according to Rule 31 of SPPRA, 2010.
- To Perform any other function ancillary and incidental to the above.

- DR. FAZLULLAH PECHUHO -
SECRETARY TO GOVERNMENT OF Sindh

No.HD(P&E)3-2(427)/2014.

Karachi dated the 10th APRIL, 2017

1. The D.G.Health Services, Sindh, Hyderabad.
2. The District Health Officers (All)
3. Medical Superintendents (All) *Liaquat University Hyderabad*
4. All the Member of the Committee.
5. The PS to Secretary Health Department, Govt. of Sindh, Karachi.
6. Office order file.

[Signature]
SECTION OFFICER (PM&I)

[Signature]

[Signature]
24/4
Gen B:

TENDER NOTICE

- 1) According SPPRA Rules 2010 (Amendment-2013) sealed tender on prescribed proforma are hereby invited from well reputed firms, interested agent / Sole Agent/ Foreign Companies Distributors in Pakistan for the purchase of Machinery / Equipment for Liaquat University Hospital, Hyderabad/Jamshoro for the financial year 2017-18. The last date for submission of tender documents is 27th March, 2018 up to 11.30 A.M and will be opened on same day at 12.00 Noon in the presence of participants.

Tender Enquiry No.	40/2017-18 & 41/2017-18
40/2017-18	Purchase of Laundry Machine with Accessories Under SNE 2017-18
41/2017-18	Purchase of Machinery / Equipment for (RESCUE CENTRE) Neuro- Surgery Department (PART-II), LUH, Hyderabad) Under ADP/SNE 2017-18
Bidding Procedure	Single Stage Two Envelope
Bid Security	2.5% of the total bid value
Bid Validity	90 days
Tender Fee	Rs 2,000/- each (non-refundable)
Issuance of Tender Documents	07.03.2018 to 26.03.2018 @ LUH, Hyderabad
Submission of Tender	27.03.2018 at 11:30 Noon @ LUH, Hyderabad
Opening of Tender	27.03.2018 at 12:00 pm @ LUH, Hyderabad

- 3) Complete set of tender documents containing Schedule of Requirements, Technical Specification with Term & Conditions can be purchased with a non-refundable fee in Rs 2,000/- Cash from the office of undersigned Liaquat University Hospital (LUH), Hyderabad.
- 4) The Medical superintendent LUH, Hyderabad / Jamshoro reserves the right to increase or decrease the quantity of any item of schedules as and when it is deemed necessary according to SPPRA Rules. The Procuring agency may reject all any bids subject to the relevant provision of SPPRA Rules.
- 5) Tender documents can be download from SPPRA website.
- 6) Bid shall include all government taxes (if applicable)
- 7) Deduction in the bills will be done as per government rules.
- 8) Bid Security @ 2.5% of the total bid value of quoted items is to be submitted by the bidders in shape of pay order / demand draft in favour of Medical Superintendent Liaquat University Hospital Hyderabad / Jamshoro whereas an amount of the contract 5% performance security is to be obtained from contractor as per SPPRA Rules.
- 9) In case of discrepancies between the Tender Notice and the Tender Documents, the Tender Documents shall take precedence.
- 10) In case of announcement of public holiday or any favorable circumstance, the bids shall be submitted and opened as per given schedule on the next working day.
- 11) Queries can be addressed at the following numbers or in person during office hours @ LUH, Hyderabad.

Ph: 022-9210207
Fax: 022-9210208
INF-KRY No. 1268/18

Medical Superintendent
Liaquat University Hospital
Hyderabad

ہم دشمنی کے خلاف متحد ہیں۔
8398

Say No to Corruption

ٽينڊر نوٽيس

1. ايس بي بي آري رولز 2010 (2013 بر ترميم ٿيل) تحت فنانشل سال 18-2017 لاءِ لياقت يونيورسٽي اسپتال حيدرآباد/ ڄامشورو لاءِ مشينري/ ايڪيوريمينٽس جي خريداري لاءِ ساڪ وارين فرمن، دلچسپي رکندڙ ايجنٽن/ سول ايجنٽن/ فارين ڪمپنين جي پاڪستان ۾ ڊسٽريبيوٽن کان مقرر يروفارما تي مهربند ٽينڊر گهريل آهن ٽينڊر دستاويز جمع ڪرائڻ جي آخري تاريخ 27 مارچ، 2018 تي 11:30 وڳي صبح تائين آهي، جيڪي ساڳئي ڏينهن 12:00 وڳي منجهند جو شرڪت ڪندڙن جي روبرو ڪوٺيا ويندا.

2

ٽينڊر انڪوائري نمبر،	41/2017-18 & 40 /2017-18
40/2017-18	ايس اين اي 2017-18 تحت لائبري مشين ساڻ اسيسٽنٽس جي خريداري
41/2017-18	اي ڊي بي/ ايس اين اي 2017-18 تحت (ريسڪيور سينٽر) نيرو سرجن ڊپارٽمينٽ لاءِ مشينري/ ايڪيوريمينٽس جي خريداري (پارٽ II) ايل يو ايج حيدرآباد.
واڪ جمع طريقي،	سنگل اسٽيج پڻ لڳا
واڪ سيڪيورٽي،	ڪل واڪ ويليو جو 2.5 سيڪڙو
واڪ جي گبوليت،	90 ڏينهن
ٽينڊر ٽي،	2000 (روپيا هر هڪ (ٽو روڻ جوڳي)
ٽينڊر دستاويز جاري ڪرڻ،	07-03-2018 کان 26-03-2018 تائين ايل يو ايج حيدرآباد ۾
ٽينڊر جمع ڪرائڻ،	27-03-2018 تي 11:30 وڳي صبح ايل يو ايج حيدرآباد ۾
ٽينڊر کولڻ،	27-03-2018 تي 12:00 وڳي منجهند ايل يو ايج حيدرآباد ۾

- ٽينڊر دستاويزن جو مڪمل سيٽ ساڻ گهرجن جو شيڊيول، تصريحات، شرطن ۽ شروطن سميت 2000 روپيا نه روڻ جوڳي ٿي روڪ ادا ڪري هيٺ صحيح ڪندڙ جي آفيس لياقت يونيورسٽي اسپتال (ايل يو ايج) حيدرآباد مان خريد ڪري سگهجي ٿو.
- ايس بي بي آري رولز تحت ميڊيڪل سپرنٽينڊنٽ ايل يو ايج حيدرآباد / ڄامشورو کي اختيار آهي ته جڏهن ۽ جتي به ضروري سمجهي ته اسمن جو تعاد گهٽائي يا وڌائي، پروڪيورنگ ايجنسي ايس بي بي آري رولز جي لاڳاپيل شقن تحت ڪري يا سمورا واڪ رد ڪري سگهي ٿي.
- ٽينڊر دستاويز ايس بي بي آري ويب سائيٽ تان به ڊائون لوڊ ڪري سگهجن ٿا.
- واڪن سان (لاڳو هجڻ) نه سمورا سرڪاري ٽيڪس شامل ڪرڻا پوندا.
- بلن مان سرڪاري قاندين موجب ڪوتاهي ٿيندي.
- ڪمپل اسمن جي ڪل واڪ ويليو جو 2.5 سيڪڙو واڪ سيڪيورٽي پي آرڊر/ ڊمانڊ ڊرافٽ جي صورت ۾ ميڊيڪل سپرنٽينڊنٽ لياقت يونيورسٽي اسپتال حيدرآباد/ ڄامشورو جي نالي جمع ڪرائڻي پوندي، جيئن ته معاهدي جي رقم جو 5 سيڪڙو پرفارمنس سيڪيورٽي ايس بي بي آري رولز تحت نيڪيڊار پاران حاصل ڪئي ويندي.
- جيڪڏهن ٽينڊر نوٽيس ۽ ٽينڊر دستاويزن وچ ۾ ڊسڪريپنسي ٿي ته ٽينڊر دستاويزن کي طريقي تحت اڪلائو ويندو.
- جيڪڏهن سرڪار پاران عام موڪل جو اعلان ٿيو يا ڪا اڻ ٿيڻي صورتحال ٿي ته واڪ ٻئي ڪر واري ڏينهن جا ٿايل شيڊيول تحت جمع ڪرائي ڪوٺيا ويندا.
- ڪنهن به معلومات لاءِ آفيس وقت دوران هيٺ ڄاڻايل نمبرن تي يا ايل يو ايج سان رابطو ڪريو.

فون: 022-9210207، فيڪس: 022-9210208




ميڊيڪل سپرنٽينڊنٽ
لياقت يونيورسٽي اسپتال حيدرآباد

INF/KRY No:1268/2018



March 08 2018
Daily Iqbal

MEETING OF PROCREMENT COMMITTEE FOR OPENING OF TENDER DOCUMENTS FOR PURCHASE OF MACHINERY / EQUIPMENT RESCUE PART-II (NEURO-SURGERY) FOR THE FINANCIAL YEAR 2017-18 AT LIAQUAT UNIVERSITY HOSPITAL, HYDERABAD/ JAMSHORO IN THE COMMITTEE ROOM LUH, HYDERABAD ON 27.03.2018.

S.NO	NAME & DESIGNATION		SIGNATURE
01	Dr. Naeem Zia Memon Addl: Medical Superintendent (General). LUH, Hyderabad.	Chairman	
02	Prof. Raja Riaz Ahmed Head of Neuro-Surgery Department LUMHS, Jamshoro	Member	
03	Dr. Anjum Rehman Addl: Medical Superintendent (Technical). LUH, Hyderabad.	Member	

Opening of Tender Documents for Purchase of Machinery / Equipment (PART-II) RESCUE CENTRE (NEURO-SURGERY) UNDER SNE /ADP
for the Financial year 2017-18 at Liaquat University Hospital, Hyderabad/Jamshoro

ATTENDANCE SLIP

S.No.	Name of Firm	Phone Number	Postal Address	Name of Participant	C.N.I.C No: of participants	Signature
01	Endo-Kare	0341-8735179	SECTOR P.E.C.H.S 86-2 KARACHI	Rasheed Ahmed	42201-4582987-7	
02	BIOS	0333-2724054	Karachi	Muhammed farooq	41303894962294	
03	Tasani Scientifics		KHI/F-14D	Abdul Bari	4130434262525	
04	Allmed Selections	0333-2753119	Karachi	Abdul-Ala-Stray	41303-6967844-5	
05	Laf Brothers Instruments	0334-2688495	KARACHI.	FARAZ UDDIN SHAIKH	41304-4870363-7	
06	Verizon	03422438328	Karachi	Faiz Ullah	42201-1789218-3	
07	Eastern Optical	0342-3347055	Karachi	Tunaid	42501-121424-3	
08						

(Dr. Naeem Zia Memon)
Addl: Medical Superintendent (General)
LUH, Hyderabad
Chairman Procurement Committee

(Dr. Anjum Rehman)
Addl: Medical Superintendent (Tech)
LUH, Hyderabad
Member Procurement Committee

(Prof. Raja Riaz Ahmed)
Head of Neuro-Surgery Department
LUMHS, Jamshoro
Member Procurement Committee

MINUTES OF BID OPENING MEETING

NIT No.	Inf No:1268/2018
SPPRA Number	S.No: 37150
Method of Procurement	Single Stage Two Envelope

Name of Work: **Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department (Part-II) At LUH, Hyderabad)**


Meeting of the Procurement Committee (PC) was held on Tuesday, 27March 2018 for opening of above mentioned NIT. Meeting was attended by members of the Procurement Committee and the representatives of bidder (attendance sheets are enclosed).

The following companies purchased bidding documents after advertisement of the tender notice till deadline:


- 1) M/s. Allmed Solution
- 2) M/s. Verizon
- 3) M/s. Endocare
- 4) M/s. Jassani Scientific
- 5) M/s. Eastern Optical Company
- 6) M/s. Latif Brothers
- 7) M/s. BIOS

The following company participated in the bidding process with its respective bidby submission deadline of 11:30 AM on Tuesday 27.03.2018.


- 1) M/s. Allmed Solution
- 2) M/s. Verizon
- 3) M/s. Endocare
- 4) M/s. Jassani Scientific
- 5) M/s. Eastern Optical Company
- 6) M/s. Latif Brothers
- 7) M/s. BIOS



(Chairman)
Dr. Naem Zia Memon
Addl: Medical Superintendent (Gen)
Liaquat University Hospital
Hyderabad



(Member)
Dr. Riaz Ahmed Raja
Head of Neurosurgery Department
LUMHS
Jamshoro





(Member)
Dr. Anjum Rehman
Addl: Medical Superintendent
Liaquat University Hospital
Hyderabad

**PROCUREMENT COMMITTEE
ATTENDANCE SHEET**

Tender No. 41/2017-18Name of Work: **Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18
(Rescue Centre) Neuro- Surgery Department (Part-II) At LUH, Hyderabad)**

The following members of the Procurement Committee (PC) were present on Tuesday, 27 March 2018 for opening of above mentioned NIT.

1.	Dr. Naeem Zia Memon	Additional Medical Superintendent Liaquat University Hospital Hyderabad / Jamshoro	Chairman	
2.	Dr. Riaz Ahmed Raja	Head of Neuro Surgery Department LUMHS, Jamshoro	Member	
3.	Dr. Anjum Rehman	Addl: Medical Superintendent (I) Liaquat University Hospital Hyderabad	Member	

Tender No. 41/2017-18
Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
 Opened on 27.03.2018 12:00PM

PARTICIPATING BIDDERS

S. No.	Item Description	Qty	M/s Allmed Solution	M/s Verizon	M/s Endocare	M/s Jassani Scientific	M/s Eastern Optical Company	M/s Latif Brothers	M/s BIOS
1	ENDOSCOPIC SPINE SURGERY SET	1	Yes	Yes	-	-	-	-	-
2	ENDOSCOPIC TRANS SPHENOID SURGERY SET	1	Yes	-	-	-	-	-	-
3	THIRD VENTRI COLOSTOMY ENDOSCOPIC SURGERY SET	1	Yes	-	-	-	-	-	-
4	CAMERA CONTROL UNIT	1	Yes	Yes	Yes	-	-	-	-
5	NEURO-SURGERY MICROSCOPE	1	-	-	-	Yes	Yes	Yes	-
6	SURGICAL PRISMATIC LOUPE/MAGNIFICATIONS OF 3.5X. WORKING DISTANCE'S 46CM THESE LOUPES ARE HIGHERMAGNIFICATION WITH PRISMATIC OPTICS.	1	-	-	-	-	-	Yes	-
7	INTERA OPERATIVE NERVE MONITORING SYSTEM 8-CHANNEL	1	-	-	-	-	-	-	-
8	HIGH SPEED NEUROSURGERY ELECTRIC DRILL SYSTEM	1	Yes	-	-	-	-	-	-
9	ULTRASONIC SURGICAL ASPIRATOR (CUSA)	1	-	-	-	-	-	-	Yes
10	NEURO NAVIGATION SYSTEM	1	-	-	-	-	-	-	-

(Chairman)

Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad

(Member)

Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro

(Member)

Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad


Tender No. 41/2017-18
Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad
 Opened on 27.03.2018 12:00PM

DOCUMENTS CHECKLIST

S. No.	Requirements of Document / Pre-requisite	M/s Allied Solution	M/s Verizon	M/s Endocare	M/s Jassani Scientific	M/s Eastern Optical Company	M/s Latif Brothers	M/s BIOS
(a)	Tender Purchase Receipt (original)	Yes	Yes	Yes	Yes	No.	Yes	Yes
(b)	Bid Security	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(c)	General & Special Conditions of Contract (duly filled, signed & stamped by Bidder)	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(d)	Schedule of Requirements & Technical Specifications (duly filled, signed & stamped by Bidder)	Yes	Yes	Yes	No	No	Yes	Yes
(e)	Manufacturer's Authorization	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(f)	Undertaking	Yes	Yes	Yes	Yes	No	Yes	Yes
(g)	Certificate	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(h)	Bidder's registration & membership with a valid copy of:							
	(i) Income Tax & GST Registration Certificate	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	(ii) Professional Tax Certificate (Sindh)	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(i)	Bidder's Financial Status:							
	(i) Company Profile	Yes	Yes	Yes	Yes	No	Yes	Yes
	(ii) Bank Certificate	Yes	Yes	Yes	Yes	No	Yes	Yes
	(iii) Income Tax Return for annual business of 10 million rupees or more (turn-over (last three years))	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(j)	Bidder's After Sale Services in Sindh:							
	(i) Service Workshop	Yes	Yes	Yes	Yes	No	Yes	Yes
	(ii) Tools List	Yes	Yes	Yes	No	Yes	Yes	Yes
	(iii) Qualified & Trained Personnel List	Yes	Yes	Yes	Yes	Yes	Yes	Yes
(k)	Original Equipment Manufacturer (OEM) or Brand quoted by the Bidder							

[Signature]

S. No.	Requirements of Document / Pre-requisite	M/s Ahmed Solution	M/s Verizon	M/s Endocare	M/s Jassani Scientific	M/s Eastern Optical Company	M/s Latif Brothers	M/s BIOS
	(i) Brochure or Catalogue (Original) [Note: Photocopies, Photographs or Word document not acceptable.]	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	(ii) References in Sindh & Pakistan	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	(iii) ISO 9001 Certificate	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	(iv) ISO 13485 Certificate (where applicable)	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	(v) CE / FDA / JIS Certificate	Yes	Yes	Yes	Yes	Yes	Yes	Yes
	REMARKS	Responsive	Responsive	Responsive	Not Responsive	Not Responsive	Responsive	Responsive



(Chairman)

Dr. Naeem Zia Memon


Addl: Medical Superintendent (Gen)
Liaquat University Hospital
Hyderabad



(Member)

Dr. Riaz Ahmed Raja

Head of Neurosurgery Department
LUMHS
Jamshoro



(Member)

Dr. Anjum Rehman

Addl: Medical Superintendent
Liaquat University Hospital
Hyderabad

Tender No. 41/2017-18


**Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)**


Opened on 27.03.2018 12:00PM


BIDDERS ELIGIBILITY EVALUATION

S. No.	Parameter	Max Points	M/s Allmed Solution	M/s Verizon	M/s Endocare	M/s Jassani Scientific	M/s Eastern Optical Company	M/s Latif Brothers	M/s. BIOS
1	Conformity to the Technical Specifications	20							
	a) Fully compliant with the required specifications	20	20						
	b) Compliant with minor deviation ≤10% (subject to main function is not affected)	15		15	0	15	15	15	15
2	Warranty	20							
	a) Warranty (period more than required)	20							
	b) Warranty (period as required)	15	15	15	15	15	15	15	15
3	Bidder's Legal Status, Certification & Experience	15							
	a) NTN & GST Certificate	2	2	2	2	2	2	2	2
	b) Professional Tax Certificate	2	2	2	2	2	2	2	2
	c) SECP Incorporation Certificate	2	0	0	0	0	0	0	0
	d) ISO 9001 Certificate	1	1	1	1	0	1	0	1
	e) Purchase Orders of last year worth ≥ 1 million rupees (2 point/each order copy)	8	6	6	2	4	4	6	8
4	Bidder's Financial Status	9							
	a) Bank Certificate	3	3	3	3	3	0	3	3
	b) Income Tax Return	3	3	3	3	3	0	3	3
	c) Audited Financial Statement	3	3	3	3	3	0	3	3
5	Bidder's After Sales Services in Sindh	6							
	a) Service Workshop	3	3	3	3	3	0	3	3
	b) Qualified & Trained Personnel (BE/BSc/DAE) with Bio-Data	3	3	2	2	2	0	2	3

S. No.	Parameter	Max Points	M/S Allmed Solution	M/S Verizon	M/S Endocare	M/S Jassani Scientific	M/S Eastern Optical Company	M/s Latif Brothers	M/S. BIOS
6	Original Equipment Manufacturer (OEM) or Brand Quoted	30							
a)	Manufacturer's Authorization	5	5	5	5	5	0	5	5
b)	Manufacturer's Website	2	2	2	0	0	2	2	2
c)	Brochure or Catalogue (original)	2	2	2	2	2	2	2	2
d)	ISO 9001	2	2	2	2	2	2	2	2
e)	ISO 13485	2	2	2	2	2	2	2	2
f)	CE	2	2	2	2	2	2	2	2
g)	FDA	4	4	4	0	0	0	0	4
h)	JIS	2	0	0	0	0	0	0	0
i)	References of OEM brand / model								
(i)	Government / Semi-Government Teaching Hospital / Institute	3	3	2	2	2	2	2	2
(ii)	Armed Forces / NGOs Hospital / Institute	2	0	0	0	0	0	0	2
(iii)	Private Renowned Teaching Hospital / Institute	2	0	2	0	0	0	0	2
(iv)	International Hospital / Institute	2	2	0	0	0	0	0	2
	Total Points	100	85	78	51	67	51	71	85
			Eligible	Eligible	Ineligible	Ineligible	Ineligible	Eligible	Eligible


 (Chairman)
Dr. Naem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad


 (Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro


 (Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18
 Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
 (Part-II) At LUH, Hyderabad)
 Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
 COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUIREITE**

S. No.	Item Description	Qty	M/s Allmed Solution	M/s Verizon
1	ENDOSCOPIC SPINE SURGERY SET	01	KarlStorz SC&CO KG Germany	Richard wolf Germany
	Telescope 25°, eyepiece angles 90°,Diameter 4mm, Length 9 cm 1		Yes	Yes
	Trocar 23mm diameter 1		Yes	Yes
	Telescope 25°, eyepiece angles 90°,Diameter 4mm, Length 11 cm 1		Yes	Yes
	Trocar 23mm diameter 1		Yes	Yes
	Attachment for 23 mm Trocar 1		Yes	Yes
	Optic Holder 23mm 1		Yes	Yes
	Puncture Needle, including stylet, diameter 1.7 mm, working length 18cm, with 1.4 mm opening for guidewire, 1		Yes	Yes
	Guide wire, not sterile, diameter 1.2mm, length 31 cm, package of 10 1		Yes	Not mentioned
	Dilation Sleeve, OD5.2mm, ID 1.5mm, graduated, length 23cm 1		Yes	Yes
	Dilation Sleeve, OD8.9 mm, ID 5.3mm, graduated, length 21 cm 1		Yes	Yes
	Dilation Sleeve, graduated, outerdiameter 12.7 mm, inner diameter 9.0 mm, length 19 cm 1		Yes	Yes
	Dilation Sleeve, OD14.9mm, ID12.9mm, graduated, length 17cm 1		Yes	Yes
	Dilation Sleeve, OD16.9 mm, ID15.1mm, graduated, length 15cm 1		Yes	Yes
	Dilation Sleeve, OD18.9 mm, ID17.1mm, graduated, length 14 cm 1		Yes	Yes
	Dilation Sleeve, OD20.9 mm, ID19mm, graduated, length 13 cm 1		Yes	Yes
	Bone Punch 40°, upbitingforward,size 4 mm, working length 24 cm 1		Yes	Yes
	Bone Punch 40°, upbitingforward,size 2 mm, working length 24 cm 1		Yes	Yes
	Spoon Forceps, dismountable, robust, oval, single action jaws,spoon size 3 x 10 mm, working length 20 cm 1		Yes	Yes
	Spoon Forceps, dismountable, curved 30°, robust, oval, spoon size 3 x 10 mm, single action jaws, 1 working length 20 cm		Yes	Yes

[Handwritten Signature]


[Handwritten Signature]


S. No.	Item Description	Qty	M/s Allmed Solution	M/s Verizon
1	ENDOSCOPIC SPINE SURGERY SET	01	KarlsStorz SC&CO KG Germany	Richard wolf Germany
	Hook Scissors, single action jaws, size 2.7 mm, working length 25 cm 1		Yes	Yes
	Surgical handle, bayonet-shaped with working length 15 cm, 1		Yes	Yes
	Bipolar Coagulating Forceps, insulated, bayonet-shaped, tip 1.2 mm, length 23 cm 1		Yes	Yes
	Palpation Hook, straight, distally 10 mm long and 90° angled, with ball, working length 20 cm 1		Yes	Yes
	Dissector dead hand, bayonet shaped, 3 mm, curved upwards, with round handle, sharp, working length 16 cm 1		Yes	Yes
	Nerve retractor, 30° angled, distal width 5 mm, working length 17 cm 1		Yes	Yes
	Curette, small, curette size (l x w): 2.7 x 4 mm, bajonet-shaped, distal angled 45°, working length 20 cm 1		Yes	Yes
	Suction Tube, with cut-off hole and stylet, working length 15 cm, 2.5 mm 1		Yes	Not mentioned
	Suction Tube, with distal nerve retractor, with cut-off hole, with adaptor, diameter 2.7 mm, working length 15 cm 1		Yes	Yes
	Rotation Socket to clamp on the operating table with one already mounted butterflynut, for use with European and United States standard rails, with lateral clamping element for height and angle adjustment of the articulated stand 1		Yes	Yes
	Articulated Stand, reinforced version, only, L-shaped, with one mechanical central clamp for all five joint functions, height 48 cm, operating range 52 cm, with fastener: KSLock (female) 1		Yes	Yes
	Palpation Hook, hook distally angled 90°, blunt, working length 20 cm 1		Yes	Yes
	Palpation hook, distally 90° angled with ball and working length 20 cm, bayonet shaped 1		Yes	Yes
	Nerve hook, distally 5mm, bajonetshaped, working length 15cm 1		Yes	Yes
	Nerve hook, distally 3mm, bajonetshaped , working length 15cm 1		Yes	Yes
	Nerve Retractor, hook 4 mm, angled sheath, working length 20 cm 1		Yes	Yes
	Elevator, sharp, slightly curved spatula, tip angled 15°, size 2 mm, with round handle, length 25 cm 1		Yes	Yes
	Bone Punch 90°, upbiting forward, size 4 mm, working length 24 cm 1		Yes	Yes
	Bone Punch 90°, upbiting forward, size 2 mm, working length 24 cm 1		Yes	Yes

Item Description

S. No.	Item Description	Qty	M/s Allimed Solution	M/s Verizon
1	ENDOSCOPIC SPINE SURGERY SET	01	KarlsStorz SC&CO KG Germany	Richard wolf Germany
	Punch, bayonet-shaped, downbiting 40° forward, size 2 mm, working length 17 cm 1		Yes	Yes
	Punch, bayonet-shaped, upbiting 40° forward, size 2 mm, working length 17 cm 1		Yes	Yes
	Punch, bayonet-shaped, single action jaws, movable jaw opening upwards, diameter 3.5 mm, working length 20 cm 1		Yes	Not mentioned
	BLAKESLEY Nucleus Cutting Forceps, bayonet-shaped, tip 0.7 mm, length 23 cm 1		Yes	Yes
	Bipolar Coagulating Forceps, insulated, bayonet-shaped, tip 0.7 mm, length 23 cm 1		Yes	Yes
	Fiber Optic Light Cable, size 3.5 mm, length 180 cm 1 Bipolar High Frequency		Yes	Yes
	Plastic Container for sterilizing, applicable for hydrogen peroxid- (Sterrad-) sterilizing and for storage, perforated, with lid, for use with two rigid endoscopes, with max. working length of 200 mm. External dimensions (wxdxh): 321 x 90 x 45 Mm 1		Yes	Yes
	Plastic Container Set with accessoires. For sterilization and storage of variable sets of instruments. Consisting of A Container, double level 2 Fixation- Post Silicone Tie-Downs 1		Yes	Yes
	Surgical blades for surgical handle 2 Bipolar High Frequency Cord, 300 cm 1		Yes	Yes
	REMARKS		Responsive	Responsive


 (Chairman)
Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad


 (Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro


 (Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18

Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
Opened on 27.03.2018 12:00PM

TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUISITE

S. No.	Item Description	Qty	M/s Allmed Solution
2	ENDOSCOPIC TRANSPHENOIDAL SURGERY SET	01	KarlsStorz SC&CO KG Germany
	Suction Tube, with cut-off hole, drop-shaped, with distance markings, conical distal end, 8 Ft., working length 15 cm l		Yes
	Suction Tube, with cut-off hole, drop-shaped, with distance markings, conical distal end, 6 Ft., working length 15 cm l		Yes
	Scissors, 45° delicate, Sheath 360° rotatable, working length 18 cm l		Yes
	Forceps, very delicate, oval cupped jaws 0.9 mm, curved upwards, working length 18 cm		Yes
	Forceps, round cupped jaws, diameter 0.6 mm, extra delicate, straight, working length 18 cm l		Yes
	Miniature Grasping Forceps, serrated, straight, working length 18 cm l		Yes
	Miniature Forceps, through-cutting, with fine flat jaws, bite 1 mm, curved up, working length 18 cm l		Yes
	Miniature Forceps, through-cutting, with fine flat jaws, bite 1 mm, straight, working length 18 cm l		Yes
	Miniature Forceps, through-cutting, with fine flat jaws, bite 1 mm, curved up, working length 15 cm l		Yes
	Miniature Forceps, through-cutting, with fine flat jaws, bite 1 mm, curved up, working length 15 cm l		Yes
	Miniature Nasal Forceps, with extra fine flat jaws, through-cutting, for tissue-sparing, sheath curved 30° straight jaws, width of cut 1.5 mm, with cleaning connector, working length 13 cm l		Yes
	Hook, 90°, blunt, length 25 cm, with round handle l		Yes
	Seeker, angled 45°, with ball end, diameter mm, length 25 cm l		Yes
	Seeker, 90°, with ball end, diameter 1 mm, length 25 cm l		Yes
	Dissector, sharp, tip angled 15°, with round handle, size 2 mm, length 25 cm l		Yes
	Dissector, sharp, slightly curved spatula, tip angled 15°, size 1 mm, with round handle, length 25 cm l		Yes
	Micro Respiratory, single curved to left, width 2 mm, length 25 cm l mm, length 25 cm l		Yes
	Curette, round wire, ID 3 mm, tip angled 45°, with round handle, length 25 cm l		Yes
	Ring- Curette, round wire, ID 3 mm, tip laterally angled 90°, with round handle, length 25 cm l		Yes
	Curette, round spoon, tip slightly angled, size 2 mm, with round handle, length 25 cm		Yes
	Curette, round spoon, tip slightly angled, size 3 mm, with round handle, length 25 cm		Yes

Tender No. 41/2017-18


Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUIREITE**

S. No.	Item Description	Qty	M/s Allmed Solution
3	THIRD VENTRI COLOSTOMY ENDOSCOPIC SURGERY SET	01	KarlsStorz SC&CO KG Germany
	Ventriculoscope Telescope 6°, angled eyepiece, outer diameter 6.1 mm, length 18 cm, working channel diameter 2.9 mm, irrigation/suction channel diameter 1.6, autoclavable, fiber optic light transmission incorporated. 1		Yes
	Operating sheath for ventriculoscope outer diameter 6.8 mm, working length 13.3cm 1		Yes
	Obturator 1		Yes
	Scissors, single action jaws, pointed, diameter 2mm, working length 30 cm, withoutratchet 1		Yes
	Biopsy forceps, both jaw parts movable, O 2.0mm, working length 30 cm, without ratchet. 1		Yes
	Click Line Ventriculostomy Forceps, diameter 2.0mm, working length 30 cm,without ratchet 1		Yes
	Grasping Forceps with teeth, 2.0 mm, working length 30 cm, without ratchet. 1		Yes
	Click Line Biopsy Forceps, single action jaw part, 2.7 mm o, working length 30 cm.without ratchet.1		Yes
	Biopsy Forceps, double action jaws, flexible, diameter 1 mm, working length 30 cm 1		Yes
	Ventriculostomy Forceps, diameter 1.0 mm, flexible, working length 30 cm 1		Yes
	Coagulating Electrode, bipolar, 5 Ft. 1		Yes
	Adaptor, autoclavable, facilitates changing of telescopes in sterile conditions 1		Yes
	Holding System, autoclavable 1		Yes
	Bipolar Forceps, long, flat jaws, outer diameter 2.4 mm, for single use, package of 5		Yes
	Bipolar Forceps Insert, with flat jaws, for single use, package of 5 1		Yes
	Balloon Catheter, O.D. 1.0 mm, length 40 cm, volume 0.20 ml, sterile, single use. 10pieces 1		Yes
	Knife, outer diameter 2.7 mm, working length 30 cm, consisting 1		Yes
	Bipolar High Frequency Cord 1		Yes
	Bipolar High Frequency Cord with 2 x 4 mm banana-plug 1		Yes
	Plastic Container for Sterilizing and Storage Two level 1		Yes
	Ventriculoscope 30°, angled eyepiece, outer diameter 6.1 mm, length 18 cm, working channel		Yes

[Handwritten Signature]

S. No.	Item Description	Qty	M/s Allied Solution
3	THIRD VENTRI COLOSTOMY ENDOSCOPIC SURGERY SET diameter 2.9 mm, irrigation/suction channel diameter 1.6, autoclavable, fiber opticlight transmission incorporated. 1 Operating sheath for ventriculoscope 30° outer diameter 6.8 mm, working length 13.3 cm 1	01	Karl'sStorz SC&CO KG Germany Yes Yes Yes
REMARKS			
Responsive			



(Chairman)
Dr. Naeem Zia Memon
Addl: Medical Superintendent (Gen)
Liaquat University Hospital
Hyderabad



(Member)
Dr. Riaz Ahmed Raja
Head of Neurosurgery Department
LUMHS
Jamshoro



(Member)
Dr. Anjum Rehman
Addl: Medical Superintendent
Liaquat University Hospital
Hyderabad

Tender No. 41/2017-18

Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
(opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUIREISE**

S. No.	Item Description	Qty	M/s Allmed Solution	M/s. Verizon
4	CAMERA CONTROL UNIT	01	KarlsStorz SC&CO KG Germany	Richard wolf - Germany
	Full Modular Camera System for both Flexible & Rigid endoscopy. Camera System (CCU & Camera head) should be Full HD 1920 x 1080p or better and should have backward and forward compatibility and modularity for futures upgrade and with latest image enhancement modules for better image quality and identifications of the land marks and pathology for better outcomes of the surgery.		Yes	Yes
	Full HD 1080p Video Processor CCU with integrated documentation functions for image and video capturing with Three chip full HD camera 11 leads with following technical data or Better or Equivalent Connections :- 2 x DVI-D . 1 x 3G-SDI output , 4 USB Connection (2 x front , 2 back) 3 Link connections or better or equivalent		Yes	Yes
	Max. Resolution :- 1920 x 1080p		Yes	Yes
	Power Supply :- 100-120 VAC, 50/50 Hz, 200-240 VAC, 50/60 HZ.		Yes	Yes
	Power Consumption :- 62 VA		Yes	Yes
	Power cable :- 300 cm or better		Yes	Yes
	DVI-D cable :- 300 cm or better		Yes	Yes
	Silicone Keyboard with Touch pad		Yes	Yes
	USB flash Drive :- 32 GB or Better		Yes	Yes
	Should contains following image enhancement modes:		Yes	Yes
	Homogenous illumination across the screen and dark spaces are brightened dynamically		Yes	Yes
	Enhances the color contrast, without altering the users natural color perception. Structures are represented more clearly		Yes	Yes
	Homogenous illumination and color contrast can be used together.		Yes	Yes
	Spectral change can be performed to identify tumors and normal tissues. Color change is due to spectral color shifts and color exchange.		Yes	Not mentioned
	Picture-in Picture mode control via camera head buttons		Yes	Yes

[Handwritten signature]


S. No.	Item Description	Qty	M/s Allied Solution	M/s. Verizon
4	CAMERA CONTROL UNIT	01	KarlsStorz SC&CO KG Germany	Richard wolf-Germany
	Control of peripheral devices i.e. light source,insufflator, recording system parameter via camera head buttons or better		Yes	Yes
	Still image capturing in Full HD Quality (JPEG)		Yes	Yes
	Format via camera head buttons		Yes	Yes
	Video Capturing in Full HD Quality (MPEG4 Format) via Camera head buttons		Yes	Yes
	Grid and pointer mode for teaching and training purpose or Better		Yes	Yes
	Image rotation 180 degree via camera head buttons		Yes	Yes
	20 individual preset or better		Yes	Yes
	20 Patient data back up or better		Yes	Yes
	Should have compatibility with future upgrade like with Flexible Scope, or 3D or Equivalent		Yes	Yes
	Pointer and grid option should be available		Yes	Yes
	Laparoscopic and flexible endoscopy view can be displayed on same monitor		Yes	Yes
	Full HD 3-Chip CCD Camera Head		Yes	Yes
	Three-Chip FULL HD Camera Head, compatible, progressive scan, soakable, gas- and plasma-sterilizable, with integrated Parfocal Zoom Lens, focal length f – 15 – 31 mm (2x), 2 freely programmable camera head buttons		Yes	Yes
	Image sensor: 3 x 1/3 " CCD chip		Yes	Yes
	Pixels: 1920 (h) x 1080 (v) pixels per chip.		Yes	Yes
	Sensor type: CCD chip		Not mentioned	Yes
	Aspect Ratio: 16:9		Yes	Yes
	Progressive scan (full frame) for Integrated zoom lens f= 15-31 mm (2x optical zoom).		Yes	Yes
	Display of 50 or 60 frames per second. Lens:		Yes	Yes
	Minimum light sensitivity: 1.17 Lux (f = 1.4 mm).		Yes	Yes
	Control buttons: 3 (2 of them freely programmable).		Yes	Yes
	Three-chip technology for brilliant images.		Yes	Yes
	Image acquisition in format 16:9, with 1920 x 1080 pixels and progressive scan 50 Hz or 60Hz.		Yes	Yes
	Digital through and through: Conversion of optical images to digital signals at the earliest possible site:		Yes	Yes
	The CCD sensing chip.		Yes	Yes
	Zoom : Optical (2x) , Digital Zoom Through The		Yes	Yes
	Monitor In 5 Levels		Yes	Yes


[Handwritten signature]


[Handwritten signature]

Liaquat University Hospital Hyderabad / Jamshoro

S. No.	Item Description	Qty	M/s Allmed Solution	M/s. Verizon
4	CAMERA CONTROL UNIT	01	KarlsStorz SC&CO KG Germany	Richard wolf Germany
	27" Medical Grade Monitor		Yes	Yes
	27" Medical Grade Monitor from the same manufacturer and should have recommendation for endoscopic MIS surgery with following technical data. Color systems		Yes	Yes
	REMARKS		Responsive	Responsive


 (Chairman)
Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad


 (Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro


 (Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18

**Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)**
Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUISITE**

S. No.	Item Description	Qty	M/s Latif Brothers
5	NEUROSURGERY MICROSCOPE	01	OPMI-Vario S-88 Carl Zeiss Germany
	Optical head having swivable and tiltabe suspension for effortless positioning in all directions via programmable ergonomic hand grip for control of functions and release / locking of magnetic brakes		Yes
	A pochromatic optics		Yes
	Motorized zoom magnification ratio 1:6		Yes
	Motorized internal focusing from 200 to 400mm via front lens		Yes
	Coaxial fiber optic illumination		Yes
	Laser compatible		Yes
	Dust Cover		Yes
	Tiltable and retractable binocular tube with IPD adjustment		Yes
	Mobile floor stand with rotatable joint arms		Yes
	Magnetic brake system		Yes
	180W xenon illumination with adjustable brightness and quick changover to integrated back-up identical xenon lamp		Yes
	Memory for personal setting of various surgeons		Yes
	Castors with brakes		Yes
	Wired multi-function foot control panel		Yes
	HD video camera		Yes
	Video Recorder		Yes
	Asepsis set		Yes
	32" LCD/ LED		Yes
	Stereo co-observation device		Yes

[Handwritten Signature]


S. No.	Item Description	Qty	M/s Latif Brothers
5	NEUROSURGERY MICROSCOPE with three axis inclination and binocular tube with wide field 10X oculars	01	OPMI-Vario S-88 Carl Zeiss Germany
	REMARKS		Responsive



(Chairman)

Dr. Naeem Zia MemonAddl: Medical Superintendent (Gen)
Liaquat University Hospital
Hyderabad


(Member)

Dr. Riaz Ahmed RajaHead of Neurosurgery Department
I.UMHS
Jamshoro


(Member)

Dr. Anjum RehmanAddl: Medical Superintendent
Liaquat University Hospital
Hyderabad

Tender No. 41/2017-18
Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
 (Part-II) At LUH, Hyderabad)
 Opened on 27.03.2018 12:00PM

TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUIREITE

S. No.	Item Description	Qty	M/s Latif Brothers
6	SURGICAL PRISMATIC LOUPESMAGNIFICATIONS OF 3.5X, WORKING DISTANCES .46CM THE SELOUPESAREHIGHER MAGNIFICATION WITH PRISMATICOPTICS	01	EyeMag Pro F, EyeMagLight-II Carl Zeiss, Germany
	Prismatic loupes are laser aligned and treated with antire flective coating to produceas open or image.		Yes
	Prismatic loupes		Yes
	Pair of protective caps		Yes
	Flip lever		Yes
	Keelers port frame		Yes
	Light weight protective shield		Yes
	2xadjustablenosepieces		Yes
	Plano prescription insert		Yes
	Neck cord		Yes
	Lens cloth		Yes
	Protective case		Yes
	LED illumination gives 34000		Yes
	Lux of homogenous white light,while coaxialillumination ensur esshadow freeviewing.		Yes
	Lithium-ion battery which will give upto7 hours continuous use before are charge is required.		Yes
	LED light system		Yes
	1xlithiumbatteryback		Yes
	Charging Unit		Yes
	Transformer		Not Mentioned
	Portable protective carry case		Yes
	REMARKS		Responsive

(Chairman)

Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital, Hyd

(Member)

Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS, Jamshoro

(Member)

Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital, Hyd

Tender No. 41/2017-18

**Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
Opened on 27.03.2018 12:00PM**

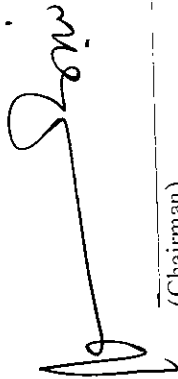
**TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUIRESITE**

S. No.	Item Description	Qty	No Bid Received for this item
7.	Intera operative Nerve Monitoring System 8-Channel Latest & advanced intera operative Nerve Monitoring System for highly advanced Head - Neck Surgeries with: A. 8 - Channel EMG Touch screen monitoring. B. Independent Stimulator. C. Clear and loud EMG signal sound. D. Glare free and clearly visible EMG signals. E. Disposable EMG monitoring electrodes and stimulator probes for minimum 25 surgeries. For: 1. Skull base Surgeries. 2. Facial Nerve Surgery. 3. Minimal Invasive Surgeries. 4. Specialty Procedures. Required Key Features: Audio / Visual data Touch - screen controls Surgeons / Procedures settings Menu driven Simulator for training and education Contextual trouble shooting CAS integration Stimulation adjustment and software control at fingertip from sterile field Current delivered tone (CDT) Microscope VGA output Stimulus" voice Event threshold	01	

[Handwritten signature]

Liaquat University Hospital Hyderabad / Jamshoro

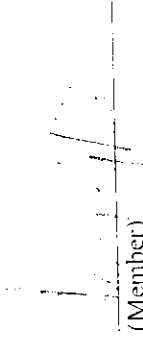
Auto event threshold			
Event capture "15s" & "60ms" screens			
200, 500, 2000uv scale			
Print			
Video output			
USB output			
Freeze			
Measurement cursor			
Largest / Latest			
Electrode check			



(Chairman)
Dr. Naem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad



(Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro



(Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18

Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
 (Part-II) At LUH, Hyderabad)
 Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
 COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUISITE**

S. No.	Item Description	Qty	Allmed Solution
8..	High Speed Neurosurgery Electric Drill System	01	KarlsStorz SC&CO KG Germany
	For Department of Neurosurgery, Advanced Drill System for surgeries like:		Yes
	Craniotomies.		Yes
	Spine Surgeries.		Yes
	Skull Base Surgeries.		Yes
	Minimal Invasive Surgeries.		Yes
	Specialty Procedures.		Yes
	Power Console:		Yes
	Input Voltage Range: 100v - 240v } 10%		Yes
	Power Supply Frequency: 50 - 60 Hz		Yes
	Power Consumption: 500 VA.		Yes
	User Friendly interface.		Yes
	Microprocessor Controlled.		Yes
	Pre-Loaded Menu Driven Software Guidance.		Yes
	Touch Screen 8 inch or more; Glare free, high resolution.		Yes
	Built-in separate Irrigation Pump.		Yes
	Built-in separate Cooling Pump.		Yes
	Emergency ON / OFF Button.		Yes
	Built-in grip for IV Pole.		Yes

S. Sarin

[Signature]

<p>Built-in support for Automated Cleaning of Endoscope Lens 2- Motor: High Torque (minimum 3.9 N cm), High Speed (up to 200 - 75000 rpm). Light weight (up to 180 grams). Low Noise (up to 58db). Ergonomically designed and Slim (length 9.02 cm, diameter 2.03 cm). Must be able to adopt more than 45 attachments of different geometry, size and functionality of End-User's choice.</p>		<p>Yes</p>
<p>Footswitch:</p>		<p>Yes</p>
<p>Advanced Control of mode selection, speed control, reverse, forward, Variable Speed, Start, Stop functions.</p>		<p>Yes</p>
<p>Optional Foot Pedal for Scrub Nurse to help the surgeon. Please quote separate price of this additional item, which must be compatible with main footswitch and console.</p>		<p>Yes</p>
<p>Color Coded Attachments (One Each with mentioned number of single use Burrs):</p>		<p>Yes</p>
<p>Small Straight Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Medium Angled Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Perforator Driver (Hudson End) with 5 cutters for burr hole.</p>		<p>Yes</p>
<p>Craniotomy Adult with total 100 cutters.</p>		<p>Yes</p>
<p>Medium Straight Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Large Straight Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Small Angled Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Large Angled Attachment with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Craniotomy Pediatric with total 50 cutters.</p>		<p>Yes</p>
<p>Metal Cutter Attachment with total 20 assorted Cutters.</p>		<p>Yes</p>
<p>MIS Tube Attachment. Straight with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>MIS Tube Attachment. Angled with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>MIS Tube Attachment. Curved with total 20 assorted Burrs.</p>		<p>Yes</p>
<p>Accessories:</p>		<p>Yes</p>
<p>Please quote all accessories needed for the quoted system including Sterilization Box, Battery backup Unit, Cleaning Brushes, lubrication spray etc.</p>		<p>Yes</p>
<p>Optional Accessories. One Each (Please quote separate prices):</p>		<p>Yes</p>
<p>Dedicated Spine Disc Shaver motorized hand piece compatible with electric System along with 25 disposable blades.</p>		<p>Yes</p>
<p>Dedicated Sinuses Shaver motorized hand piece compatible with electric System along with 30 disposable blades.</p>		<p>Yes</p>
<p>Rotating Craniotomy. Adult.</p>		<p>Yes</p>
<p>Straight Attachment of Expandable Length.</p>		<p>Yes</p>

[Handwritten Signature]


Angled Attachment of Expandable Length.	Vendor will need to supply Imported & Compatible Pure Sine Wave UPS System with built in AVR and power surge protection.	Vendors will Supply Manuals of the quoted system.	Yes
Remarks			Yes
			Responsive



(Chairman)
Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad



(Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro



(Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18

Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
(Part-II) At LUH, Hyderabad)
Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUISITE**

S. No.	Item Description	Qty	M/s. BIOS
9.	ULTRASONIC SURGICAL ASPIRATOR (CUSA)	01	Sonosca 300 Soring-Germany
	For use in different brain and spinal operations.		Yes
	Magnetostrictive technology with water cool hand pieces.		Not mentioned
	Ultrasonic Surgical Aspirator (con solc) with foot switch control system		Yes
	System capable of dual frequencies i.e. 23 KHz and 36 KHz		Yes
	Electric ultrasonic aspirating system 100 Watt output power.		Yes
	Irrigation flow maximum 25 ml to 50 ml/min.		Yes
	Suction pressure 0-0.6 bar or better		Yes
	Steam autoclavable hand pieces.		Yes
	Ultrasonic surgical aspirator system on mobile trolley with 4-wheel castors		Yes
	Variable dual energy / frequencies and control aspiration		Yes
	Tissue selection mode		Yes
	Integrated cooling and suction facility		Yes
	Compatible module for electrosurgical unit		Yes
	Built in irrigation pump in the unit.		Yes
	Irrigation output The irrigation rate display shows digits 1 – 10 or more		Yes
	One Hand Piece straight with resonance frequency 36 kHz.		Yes
	One Hand Piece angled with resonance frequency 23 kHz		Yes
	Sterilization case for each hand piece		Yes
	Ultrasonic bone sculpting saber tip		Yes
	Micro Tip for Transphenoidal work		Yes
	Biopsy collection Trap		Yes
	Shear Tips 4.60" length for removal of fibrous etc.		Not mentioned
	Tubing kit for irrigation system		Yes

[Handwritten signature]

[Handwritten signature]

Tubing kit for suctioning system		Yes
FDA or European Directive 93/42/EEC CE certificates CE12756		Yes
Remarks		Responsive



(Chairman)
Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad



(Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Jamshoro



(Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

Tender No. 41/2017-18

Purchase Of Machinery /Equipment Under SNE/ ADP For The Year 2017-18 (Rescue Centre) Neuro- Surgery Department
 (Part-II) At LUH, Hyderabad)
 Opened on 27.03.2018 12:00PM

**TECHNICAL EVALUATION REPORT
 COMPARATIVE STATEMENT ON COMPLIANCE AS PER TENDER REQUISITE**

S. No.	Item Description	Qty	No bid received for this item
10.	Latest &Advanced Neuro Navigation Systemalong with complete Accessories	01	
	Two Carts Dual Display System on Caster, Lockable system		
	To localize and operate on small lesion of brain with pin pointed accuracy		
	Vital role in placement of brain implants especially deep brain stimulation electrodes and implants.		
	To improves safety of the operations and reduces unnecessary neurological morbidity.		
	System must navigate with precise accuracy through Optical Navigation		
	Surgeon Cart: -		
	Surgeon Monitor (medical grade) touch screen		
	Resolution 1920 x 1080 dpi, 60Hz - 27 inch.		
	Staff Cart: -		
	Navigation visualization touch screen and camera with extended camera volume & equipped with built-in Laser Pointer for precise & hassle free centering of the camera on the field of surgery.		
	Interface for transfer of exams via CD/USB/ Networking.		
	Buy Free Operating system. Computer 8 GB Ram, 512GB SSD		
	High Graphic Processor.		
	DICOM query/retrieve compatible		
	Application Software's:		
	Cranial Software:		
	Planning & Navigation in a single Module & in		
	Main Navigation Station.		
	Software should support Planning		
	Registration in prone or any required position of the patient		

Pen

Pen

Pen

Navigation, 3D and volumetric visualization engine (volume rendering) to check and avoid vessels and probable bleeding points during surgery.			
Procedure guided software (next/back buttons) with voice prompt, instruction window and task visualization.			
The system must be equipped with brain shift and tilt correction software			
System should be able to perform following procedures:			
Frameless Brain Biopsy			
Pin Less Procedures			
Tumor resection			
Shunt Placement			
Navigated Neuro Endoscopy			
Adult & Pediatric			
Compatible with Intra-operative CT / C-arms.			
Image Merging Software for both Cranial			
To merge CT, MRI (T1, T2, Flare, Post contrast, fMRI)			
To merge & visualize multiple data sets on Navigation Station.			
Auto Merge.			
DICOM Query / Retrieve Software:			
To search, view and download patient exams directly from the hospital network to the Navigation System:			
Query of PACS systems for patient data of surgery.			
Interface for transfer of exams via CD/USB/ Networking.			
Big Free Operating system, Computer 8 GB Ram, 512GB SSD			
High Graphic Processor.			
DICOM query/retrieve compatible			
Application Software's:			
Cranial Software:			
Planning & Navigation in a single Module & in Main Navigation Station.			
Software should support Planning			
Registration in prone or any required position of the patient			
Navigation, 3D and volumetric visualization engine (volume rendering) to check and avoid vessels and probable bleeding points during surgery.			
Procedure guided software (next/back buttons) with voice prompt, instruction window and task visualization.			

SRM

[Signature]

[Signature]


The system must be equipped with brain shift and tilt correction software			
System should be able to perform following procedures:			
Frameless Brain Biopsy			
Pin Less Procedures			
Tumor resection			
Shunt Placement			
Navigated Neuro Endoscopy			
Adult & Pediatric			
Compatible with Intra-operative CT / C-arms.			
Image Merging Software for both Cranial			
To merge CT, MRI (T1, T2, flare, Post contrast, FMRI)			
To merge & visualize multiple data sets on Navigation Station.			
Auto Merge.			
DICOM Query / Retrieve Software:			
To search, view and download patient exams directly from the hospital network to the Navigation System:			
Query of PACS systems for patient data be responsibility of firm.			
Warranty: The vendor will be responsible for maintenance of the equipment including parts and service for the period of 2 years.			
Standardization: FDA or CE			
Power Supply: 220 V AC } 10%, 50 Hz			
OPTIONAL TO BE QUOTED SEPARATELY			
A. Spine Software:			
Spine software to simplify and standardize the entire planning and navigation process.			
Views for each type of CT or Fluoro-Based procedures			
(Cervical, Thoracic, and Lumbar)			
Seamless interface to a variety of C-arm Images from the C-arm should automatically be imported and be calibrated for navigation use.			
Real time tool positions overlaid onto previously acquired images.			
Spine Instruments:			
Compatible Interface for C-Arm / An interface for C-Arm 9" or 12"			
Open Spine Clamp			
Open Spine Clamp driver			
Thoracic Clamp			
Reference Frame			

h


Sen

Liaquat University Hospital Hyderabad - Janshoro


Passive Planer Ball Tip with minimum four ports of spheres				
Awl, Probe and Tap with trackers.				
B. PLANNING SOFTWARE FOR DBS PROCEDURES				
C. IMAGE FUSION SOFTWARE				
Remarks				



(Chairman)
Dr. Naeem Zia Memon
 Addl: Medical Superintendent (Gen)
 Liaquat University Hospital
 Hyderabad



(Member)
Dr. Riaz Ahmed Raja
 Head of Neurosurgery Department
 LUMHS
 Janshoro



(Member)
Dr. Anjum Rehman
 Addl: Medical Superintendent
 Liaquat University Hospital
 Hyderabad

LIAQUAT UNIVERSITY HOSPITAL

HYDERABAD / JAMSHORO

BID FINANCIAL EVALUATION REPORT

OPENED ON 24.04.2018

PURCHASE OF MACHINERY/EQUIPMENT UNDER SNE/ADP FOR THE YEAR 2017-18 (RESCUE CENTRE) NEURO-SURGERY DEPARTMENT (PART-II) AT LUH, HYDERABAD

TENDER NO. 41/2017-18

(DATED: 27.03.2018)

Enclosed:

- 1) Bid Evaluation Report**
- 2) Comparative Statement**
- 3) Meeting Minutes**

LIAQUAT UNIVERSITY HOSPITAL

HYDERABAD / JAMSHORO

BID FINANCIAL EVALUATION REPORT

OPENED ON 24.04.2018

**PURCHASE OF MACHINERY/EQUIPMENT UNDER
SNE/ADP FOR THE YEAR 2017-18 (RESCUE CENTRE)
NEURO-SURGERY DEPARTMENT (PART-II)
AT LUH, HYDERABAD**

TENDER NO. 41/2017-18









(DATED: 27.03.2018)

Enclosed:

- 1) Bid Evaluation Report**
- 2) Comparative Statement**
- 3) Meeting Minutes**

MEETING OF CENTRAL PROCUREMENT COMMITTEE FOR OPENING OF FOLLOWING FINANCIAL BIDS FOR PURCHASE OF MACHINERY / EQUIPMENT UNDER ADP / SNE FOR THE FINANCIAL YEAR 2017-18 FOR LIAQUAT UNIVERSITY HOSPITAL, HYDERABAD/ JAMSHORO HELD ON 24.04.2018 AT THE OFFICE OF VICE CHANCELLOR DOW UNIVERSITY OF HEALTH SCIENCES OJHA CAMPUS KARACHI.




1. Purchase of Machinery / Equipment for Establishment of Cardiothoracic Surgery Department at LUH, Hyderabad.
2. Purchase of Machinery / Equipment for Rescue Center (Part-I), Urology Department.
3. Purchase of Machinery / Equipment for Rescue Center (Part-II), Neuro Surgery Deptt.
4. Purchase of Laundry Machine.








S.NO	NAME & DESIGNATION		SIGNATURE
01	Professor Dr.M.Saeed Qureshi Vice Chancellor, Dow University of Health Sciences, Karachi.	Chairman	
02	Professor Dr.Tariq Rafi, Vice Chancellor, Jinnah Sindh Medical University, Karachi.	Member	
03	Professor Dr. Muneer Junejo Pro Vice Chancellor, LUM&HS. Jamshoro.	Member	
04	Professor Aneela Ataur Rehman Pro Vice Chancellor, Dean of Faculty Community Medicine, LUMHS. Jamshoro	Member	
05	Vice Chancellor, Chandka Medical University, Larkana.	Member	
06	Mr.Shafi Mohammad Qureshi Additional Director, Directorate of Pharmacy, Health Department, Government of Sindh, Karachi.	Member	
07	Additional Secretary (PM&I), Health Department, Government of Sindh, Karachi. DR. JALAL UDDIN JALALANI	Member	
08	Additional Finance Secretary, Finance Department, Government of Sindh, Karachi. MR. ATHAR Meclani	Member	
09	Additional Director NAB NAB Islamabad. MR. TAHIR	Member	

Date: 24.04.2018

Opening of Financial Bids for Purchase of Machinery / Equipment
 For Rescue Center (Part-II) Neuro Surgery Department
 Financial year 2017-18


ATTENDANCE SLIP


S.No.	Name of Firm	Phone Number	Postal Address	Name of Participant	C.N.I.C No: of participants	Signature
1	LATIF BROTHERS	0300 2024069	14. Commercial Building, The Mall Lahore	Imran	35702-2158542-3	
2	B705	0333 3631955	Kanada	RL-912200		
3	Verizon	0342243832		Farid	42201-17892183	
4						


 Member
 Member
 Member
 Member
 Member
 Member
 Chairman


BID EVALUATION REPORT


- 1) Name of Procuring Agency: Liaquat University Hospital Hyderabad / Jamshoro
- 2) Tender Reference No: 41/2017-18
- 3) Tender Description: Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18 (Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad
- 4) Method of Procurement: Single Stage Two Envelope
- 5) Tender Published: Business Recorder – Express – Ibrat
SPPRA Website S.No:37150
- 6) Total Bid Documents Sold: 07
- 7) Total Bids Received: 07
- 8) Technical Bid Opening Date: 27.03.2018
- 9) No. of Bid Technically Qualified: 04
- 10) Bid(s) Rejected: 03
- 11) Financial Bid Opening Date: 24.04.2018
- 12) Bid Evaluation Report: **Enclosed (i) Comparative Statement (ii) Minutes**



Prof. Dr. M. Saeed Qureshi
Vice Chancellor
DUHS, Karachi



Prof. Dr. Tariq Rafi
Vice Chancellor
JSMU, Karachi



Prof. Dr. Muneer Junejo
Pro Vice Chancellor
LUMHS, Jamshoro



Vice Chancellor
CMU,
Larkana


Prof. Aneela Ataur Rehman
Pro Vice Chancellor
LUMHS, Jamshoro


Mr. Shafi Mohammad Qureshi
Addl: Director, Directorate of Pharmacy
Health Department, GOS, Karachi


Additional Secretary (PM&I)
Health Department,
GOS, Karachi


Additional Finance Secretary
Finance Department, GOS,
Karachi


Additional Director NAB
National Accountability Bureau
Islamabad

Tender No. 41/2017-18

Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18 (Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad
(Dated: 27.03.2018)

Financial Bids Opened on 24.04.2018










COMPARITIVE STATEMENT

S. No.	Item Description	Qty	Bidders	Model	Make	C&F (Foreign Currency)	C&F (Equivalent to Pak Rupees)	DDP	Remarks
1	Endoscopic Spine Surgery Set	1	M/s Allmed Solution	Multiple (As per Technical Offer)	Karl Storz SE & CO KG	€ 17,728	Rs 2,403,562	Rs 2,836,480	1st Lowest
			M/s Verizon	Multiple (As per Technical Offer)	Richard Wolf	€ 35,150	Rs 4,765,637	Rs 5,510,500	2nd Lowest
2	Endoscopic Trans Sphenoid Surgery Set	1	M/s Allmed Solution	Multiple (As per Technical Offer)	Karl Storz SE & CO KG	€ 22,462	Rs 3,045,398	Rs 3,593,920	Lowest & best evaluated
3	Third Ventr Colostomy Endoscopic Surgery Set	1	M/s Allmed Solution	Multiple (As per Technical Offer)	Karl Storz SE & CO KG	€ 22,736	Rs 3,082,547	Rs 3,637,760	Lowest & best evaluated
4	Camera Control Unit	1	M/s Allmed Solution	Multiple (As per Technical Offer)	Karl Storz SE & CO KG	€ 42,289	Rs 5,733,543	Rs 6,766,240	1st Lowest
			M/s Verizon	Multiple (As per Technical Offer)	Richard Wolf	€ 43,450	Rs 5,890,951	Rs 6,810,000	2nd Lowest
5	Neuro-Surgery Microscope	1	M/s Latif Brothers	OMPI-Vario S-88	Carl Zeiss	-	-	Rs 18,750,000 18,570,000	Lowest & best evaluated
6	Surgical Prismatic Loupes Magnifications of 3.5x, Working Distances .46cm These Loupes are Higher Magnification with Prismatic Optics	1	M/s Latif Brothers	EyeMag Pro F EyeMag Light II	Carl Zeiss	-	-	Rs 548,000	Lowest & best evaluated
7	Intera Operative Nerve Monitoring System 8-Channel	1	No bid received for this item from any eligible / qualified bidder.						
8	High Speed Neurosurgery Electric Drill System	1	M/s Allmed Solution	Multiple (As per Technical Offer)	Karl Storz SE & CO KG	€ 167,106	Rs 22,656,231	Rs 26,736,960	Lowest & best evaluated

(Handwritten signatures and initials)

S. No.	Item Description	Qty	Bidders	Model	Make	C&F (Foreign Currency)	C&F (Equivalent to Pak Rupees)	DDP	Remarks
9	Ultrasonic Surgical Aspirator (CUSA)	1	M/s BIOS	Sonoca 300	Soring	€ 78,000	Rs 10,575,240	Rs 12,200,000	Lowest & best evaluated
10	Neuro Navigation System	1	No bid received for this item from any eligible / qualified bidder.						

Exchange Rate: \$: US Dollar 1 = 110.50 PKR € : Euro 1 = 137.27 PKR £ : British Pound 1 = 155.15 PKR CHF : Swiss Franc 1 = 119.14 PKR









 Prof. Dr. M. Saeed Qureshi Vice Chancellor DUHS, Karachi	 Prof. Dr. Tariq Rafi Vice Chancellor JSMU, Karachi	 Prof. Dr. Muneer Junejo Pro Vice Chancellor LUMHS, Jamshoro	 Prof. Aneela Ataur Rehman Pro Vice Chancellor LUMHS, Jamshoro	 Vice Chancellor Chandka Medical University Larkana	 Additional Finance Secretary Finance Department, GoS, Karachi	 Additional Director NAB National Accountability Bureau Islamabad
 Mr. Shafi Mohammad Qureshi Addl: Director, Directorate of Pharmacy Health Department, GoS, Karachi	 Additional Secretary (PM&I) Health Department, GoS, Karachi					

MEETING MINUTES OF THE PROCUREMENT COMMITTEE


Meeting of the Central Procurement Committee of Health Department was held on 24.04.2018 at the office of Vice Chancellor Dow University of Health Sciences Ojha Campus Karachi. Prof. Dr. M.SaeedQureshi chaired the meeting. The financial bids were opened after finalization of technical bids by the central procurement committee for Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18 (Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad.

Technical bids of Tender Enquiry No. 41/2017-18 were opened on 27.03.2018 and subsequently approved by the Procurement Committee for procurement of required items.

The following members attended the meeting:

S. No.	Name & Designation		Signature
01	Prof. Dr. M.SaeedQureshi Vice Chancellor Dow University of Health Sciences Karachi	Chairman	
02	Prof. Dr. Tariq Rafi Vice Chancellor Jinnah Sindh Medical University Karachi	Member	
03	Prof. Dr. Muneer Junejo Pro Vice Chancellor Liaquat University of Medical and Health Sciences Jamshoro	Member	
04	Prof. Aneela Ataur Rehman Pro Vice Chancellor Dean of Faculty Community Medicine Liaquat University of Medical and Health Sciences Jamshoro	Member	
05	Vice Chancellor Chandka Medical University Larkana	Member	
06	Mr. Shafi Mohammad Qureshi Additional Director, Directorate of Pharmacy Health Department, Government of Sindh, Karachi	Member	
07	Additional Secretary (PM&I) Health Department, Government of Sindh, Karachi	Member	
08	Additional Finance Secretary Finance Department, Government of Sindh, Karachi	Member	
09	Additional Director NAB National Accountability Bureau, Islamabad	Member	

Initiating the discussions, the evaluated technical data sheets of bidder was presented for perusal of the Central Procurement Committee (Copy of the Technical Evaluation Report enclosed.)



While financial evaluation, the requirement of Rule 48 of SPPRA was also observed. The financial bid of eligible and qualified firms with responsive technical offers are as under:

No.	Bidder Name	Bid Security
1	M/s Allmed Solutions	No. 01040161653 Dated: 20-03-2018 Meezan Bank Limited
2	M/s Verizon	No. 00061388 Dated: 20-03-2018 Summit Bank Limited
3	M/s Latif Brothers	No. 12116319 Dated: 21-03-2018 Allied Bank Limited
4	M/s BIOS	No. 1521000210 Dated: 26-03-2018 Al Baraka Bank Limited

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 01

Name of Item : Endoscopic Spine Surgery Set

Bidder	M/s Allmed Solution	M/s Verizon
Make	Karl Storz SE & CO KG	Richard Wolf

The offers of M/s Allmed Solutions and M/s Verizon meet all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offers of said firms were opened.

M/s Allmed Solutions offered the rates of € 17,728/- each on C&F and Rs 2,836,480/- each on DDP basis for the said item. M/s Verizon offered the rates of € 35,150/- each on C&F and Rs 5,510,500/- each on DDP basis for the said item.

The Procurement Committee approved and accepted the offer of M/s Allmed Solutions on C&F basis.

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 02

Name of Item : Endoscopic Trans Sphenoid Surgery Set

Bidder	M/s Allmed Solution
Make	Karl Storz SE & CO KG

The offer of M/s Allmed Solution meets all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s Allmed Solutions offered the rates of € 22,462/- each on C&F and Rs 3,593,920/- each on DDP basis for the said item.

The Procurement Committee approved and accepted the offer of M/s Allmed Solutions on C&F basis.

Tender No : **41/2017-18**
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : **03**

Name of Item : **Third Ventri Colostomy Endoscopic Surgery Set**

Bidder	M/s Allmed Solution
Make	Karl Storz SE & CO KG

The offer of M/s Allmed Solution meets all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s Allmed Solutions offered the rates of € 22,736/- each on C&F and Rs 3,637,760/- each on DDP basis for the said item.

The Procurement Committee approved and accepted the offer of M/s Allmed Solutions on C&F basis.

Tender No : **41/2017-18**
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : **04**

Name of Item : **Camera Control Unit**

Bidder	M/s Allmed Solution	M/s Verizon
Make	Karl Storz SE & CO KG	Richard Wolf

The offers of M/s Allmed Solutions and M/s Verizon meet all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offers of said firms were opened.

M/s Allmed Solutions offered the rates of € 42,289/- each on C&F and Rs 6,766,240/- each on DDP basis for the said item. M/s Verizon offered the rates of € 43,450/- each on C&F and Rs6,810,000/- each on DDP basis for the said item.

The Procurement Committee approved and accepted the offer of M/s Allmed Solutions on C&F basis.

Tender No : **41/2017-18**
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : **05**

Name of Item : **Neuro-Surgery Microscope**

Bidder	M/s Latif Brothers
Model	OMPI-Vario S-88
Make	Carl Zeiss

The offer of M/s Latif Brothers meets all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s Latif Brothers offered the rates of Rs ~~18,750,000/-~~ each on DDP basis for the said item.

18,570,000/-

The Central Procurement Committee approved & accepted the offer of M/s Latif Brothers on DDP basis.

Page 7 of 9

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 06
Name of Item : Surgical Prismatic Loupes Magnifications of 3.5x, Working Distances
.46cm These Loupes are Higher Magnification with Prismatic Optics

Bidder	M/s Latif Brothers
Model	EyeMag Pro F EyeMag Light II
Make	Carl Zeiss

The offer of M/s Latif Brothers meets all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s Latif Brothers offered the rates of Rs548,000/- each on DDP basis for the said item.

The Central Procurement Committee approved & accepted the offer of M/s Latif Brothers on DDP basis.

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 07
Name of Item : Intera Operative Nerve Monitoring System 8-Channel

No bid received for this item from any eligible / qualified bidder.

The Central Procurement Committee recommended to re-tender the said item.

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 08
Name of Item : High Speed Neurosurgery Electric Drill System

Bidder	M/s Allmed Solution
Make	Karl Storz SE & CO KG

The offer of M/s Allmed Solution meets all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s Allmed Solutions offered the rates of € 167,106/- each on C&F and Rs 26,736,960/- each on DDP basis for the said item.

The Procurement Committee approved and accepted the offer of M/s Allmed Solutions on C&F basis.



Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad

Item No : 09

Name of Item : Ultrasonic Surgical Aspirator (CUSA)

Bidder	M/s BIOS
Model	Sonoca 300
Make	Soring

The offer of M/s BIOS meet all the required specification and quality as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/s BIOS offered the rates of € 78,000/- each on C&F and Rs 12,200,000/- each on DDP basis for the said item.

The Central Procurement Committee approved & accepted the offer of M/s BIOS on C&F basis.

Tender No : 41/2017-18
Purchase of Machinery/Equipment under SNE/ADP for the Year 2017-18
(Rescue Centre) Neuro-Surgery Department (Part-II) at LUH, Hyderabad


Item No : 10


Name of Item : Neuro Navigation System


No bid received for this item from any eligible / qualified bidder.

The Central Procurement Committee recommended to re-tender the said item.


The meeting ended with vote of thanks from the chair.



Prof. Dr. M. Saeed Qureshi
Vice Chancellor
DUHS, Karachi



Prof. Dr. Tariq Rafi
Vice Chancellor
JSMU, Karachi



Prof. Dr. Muneer Junejo
Pro Vice Chancellor
LUMHS, Jamshoro


Vice Chancellor
CMU,
Larkana


Prof. Aneela Ataur Rehman
Pro Vice Chancellor
LUMHS, Jamshoro


Mr. Shafi Mohammad Qureshi
Addl: Director, Directorate of Pharmacy
Health Department, GOS, Karachi


Additional Secretary (PM&I)
Health Department,
GOS, Karachi


Additional Finance Secretary
Finance Department, GOS,
Karachi


Additional Director NAB
National Accountability Bureau
Islamabad

SAY NO TO CORRUPTION

Phone No: 321-9112227

No:LUH Gen-Br - 23296

Office of the
Medical Superintendent
Liaquat University Hospital
Hyderabad - Jamshoro
Dated: 21/5/2018

To,

The Managing Director,
Sindh Public Procurement Regulatory Authority,
Government of Sindh,
Karachi.

SUBJECT:- HOISTING OF BID EVALUATION REPORT.


Reference:- This office letter No:LUH Gen-Br-22571/72 Dated 16.05.2018 (Copy enclosed)

It is to submit that this office has forwarded the Bid Evaluation Report of following tenders:

1. Tender No:34 "Purchase of Machinery Equipment under ADP SNE for College Department"
2. Tender No:35 "Purchase of Machinery Equipment under ADP for Cardiovascular Surgery Department"
3. Tender No:41 "Purchase of Machinery Equipment under ADP SNE for Neuro Surgery Department"

It is added that 08 members of Procurement Committee have signed the Evaluation Report except Vice Chancellor Chandka Medical University Parkana who has proceeded abroad on Ex-Pakistan Leave.

It is therefore requested that keeping in view the cogent reasons mentioned above the Bid Evaluation Reports may kindly be hoisted on SPPRA's Website in larger public interest.


Medical Superintendent
Liaquat University Hospital
Hyderabad - Jamshoro

SPPRA INWARD DIARY

NO :

DATED : 21-05-2018

AS/16/1/18

21/5

GOVERNMENT OF SINDH
HEALTH DEPARTMENT

CORRIGENDUM

No SO(PM&I)2-1/2014(Main)/CBC. In continuation to this Department's Notification of even number dated 20-03-2018 and orders passed by Learned Judicial Commission (Water Commission) dated 22-03-2018, the Central Procurement Committee is also declared / notified as Technical Committee with the same composition. In addition to T.O.R's of Central Procurement Committee, following TORs for Technical Committee are also notified:-

TORs of Technical Committee.

- a) The Committee would be empowered to co-opt expert in case the Committee desires any assistance in any specific field.
- b) The Technical Committee shall have all the powers to procure the medical equipment, surgical equipment, machines and furniture or any other item to be installed and or fixed within the Hospital in Sindh at any level whether Tertiary, District or Taluka Hospitals.
- c) The powers of the Central Procurement Committee and the Technical Committee would extend to all the projects under the Health Department and from now onwards it would be the domain of the Committee in place of any other authority to procure medicines, furniture, instruments and machines on the ongoing projects.

DR. FAZLULLAH PECHUHO
SECRETARY HEALTH

No.SO(PM&I)2-1/2014(Main)/CBC:

Karachi dated 22nd March, 2018

A copy is forwarded for information and necessary action to:

1. The Chairman, National Accountability Bureau, Islamabad. He is requested to kindly appoint any Officer of the level of the Additional Director to be part of the Technical Committee in order to ensure transparency in the work assigned to the Committee as per orders passed by the Learned Judicial Commission (Water Commission).
2. The Registrar, Judicial Commission (Water Commission), at Honourable High Court of Sindh, Karachi.
3. The Chairman and all Members of the Committee.
4. The Secretary to Govt. of Sindh, Finance Department, Govt. of Sindh, Karachi.
5. The Managing Director, Sindh Public Procurement Regulatory Authority, Karachi.
6. The P S to Minister, Health Department, Govt. of Sindh, Karachi.
7. The P S to Secretary Health, Govt. of Sindh, Karachi.


(MUHAMMAD IBRAHIM MEMON)
DEPUTY SECRETARY (PM&I)



NOTIFICATION

No. SO (PM&I) 2-1/2014(Main)/CBC. In supersession of No. SO (PM&I) 2-1/2014(Main)/CBC of even number dated 11-08-2017 and in compliance to the order of the Hon'ble High Court of Sindh, Karachi, dated 11-08-2017 by Learned Water Commission, Central Treatment Command, Karachi, the following composition and TORs -

Composition:-

- 1 Professor Dr. Saad Qureshi, Vice Chancellor, University of Karachi, Faculty of Sciences, Karachi;
- 2 Professor Dr. Tariq Rafi, Vice Chancellor, University of Sindh, Multan, Faculty of Sciences, Karachi;
- 3 Professor Dr. Muneez Junejo, Pro. Vice Chancellor, Faculty of Health Sciences, University of Medical & Health Science, Jamshoro;
- 4 Professor Anceela Ataur Rehman, of Community Medicine, Faculty of Health Sciences, University of Medical & Health Science, Jamshoro;
- 5 Vice Chancellor, Chandka Medical University, Larkana;
- 6 Mr. Shafi Muhammad Qureshi, Additional Director, Directorate of Health Services, Pharmacy, Health Department, Govt. of Sindh, Karachi;
- 7 Additional Secretary (PM&I), Health Department, Govt. of Sindh, Karachi;
- 8 Additional Secretary (BS-19) to be nominated by Secretary, Human Resources, Govt. of Sindh, Karachi;
- 9 Additional Director, NAB to be nominated by Chairman NAB, Govt. of Sindh, Karachi.

TORs

- a) Preparing bidding documents;
- b) Carrying out technical as well as financial evaluation of the bids;
- c) Preparing evaluation report as provided in Rule 45;
- d) Making recommendations for the award of contract to the competent Authority;
- e) Perform any other function ancillary and incidental to the above;
- f) Monitoring of the procured medicines with regard to their quality and price;
- g) The Committee shall be authorized to have vigilance on distribution of the medicines in different Hospitals including all health facilities and to generate comparison chart on the website for public at large.

(DR. FAZLULLAH PECHUHO,
SECRETARY HEALTH)

No. SO (PM&I) 2-1/2014(Main)/CBC.

Karachi dated 20th March 2018.

A copy is forwarded for information and necessary action to:

- 1 The Chairman, National Accountability Bureau, Islamabad.
- 2 The Registrar Water Commission, at Honourable High Court of Sindh, Karachi.
- 3 The Chairman and all Members of the committee.
- 4 The Secretary to Govt. of Sindh, Finance Department, Govt. of Sindh, Karachi.
- 5 The Managing Director, Sindh Public Procurement Regulatory Authority, Karachi.
- 6 The P.S to Minister, Health Department, Govt. of Sindh, Karachi.
- 7 The P.S to Secretary Health, Govt. of Sindh, Karachi.

(MUHAMMAD IBRAHIM MEMON)
DEPUTY SECRETARY (PM&I)

No:LUH/Gen-Br/- 23296

Office of the
Medical Superintendent
Liaquat University Hospital
Hyderabad / Jamshoro
Dated:-21 / 05 / 2018

To,

The Managing Director,
Sindh Public Procurement Regulatory Authority,
Government of Sindh,
Karachi.

SUBJECT:- HOISTING OF BID EVALUATION REPORT.

Reference:- This office letter No:LUH/Gen-Br/-22571/72 Dated 16.05.2018 (Copy enclosed)

It is to submit that this office has forwarded the Bid Evaluation Report of following tenders:

1. Tender No:34 "Purchase of Machinery / Equipment under ADP / SNE for Urology Department".
2. Tender No:35 "Purchase of Machinery / Equipment under ADP for Cardiothoracic Surgery Department".
3. Tender No:41 "Purchase of Machinery / Equipment under ADP / SNE for Neuro Surgery Department".

It is added that 08 members of Procurement Committee have signed the Bid Evaluation Report except Vice Chancellor Chandka Medical University Larkana who has proceeded abroad on Ex-Pakistan Leave.

It is therefore requested that keeping in view the cogent reasons mentioned above the Bid Evaluation Reports may kindly be hoisted on SPPRA's Website in larger public interest.


SPPRA INWARD DIARY

NO: 2440

DATED: 22/05/2018

Ashfaq

22/5


Medical Superintendent
Liaquat University Hospital
Hyderabad / Jamshoro