

Search

Products

O.R. Integration

Surgical Light

VIDA X Series



VIDA V Series (New)

Examination Light

Suspension System


Video Solutions

Surgical Light

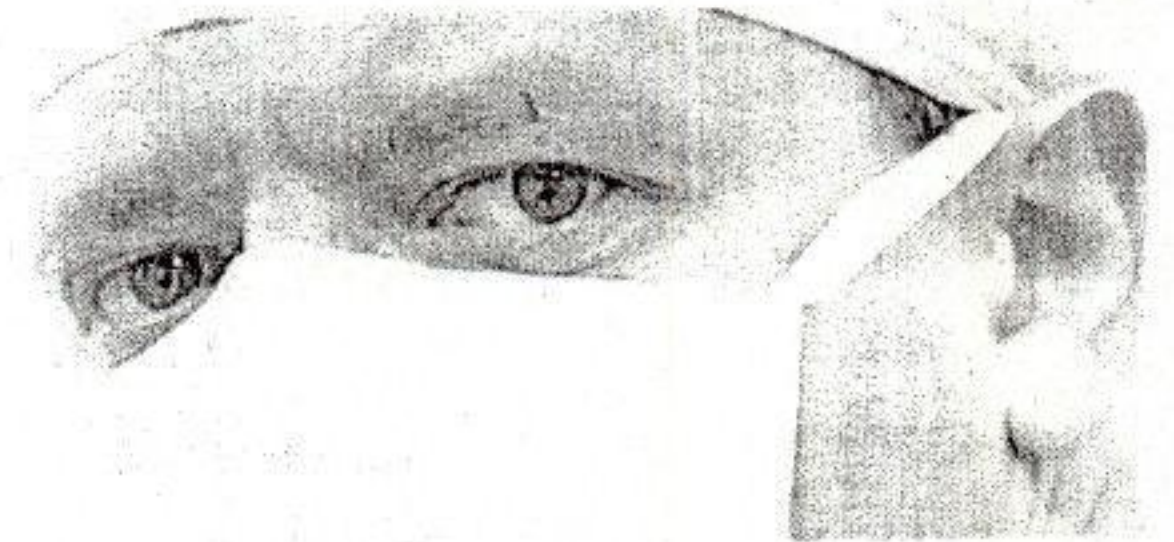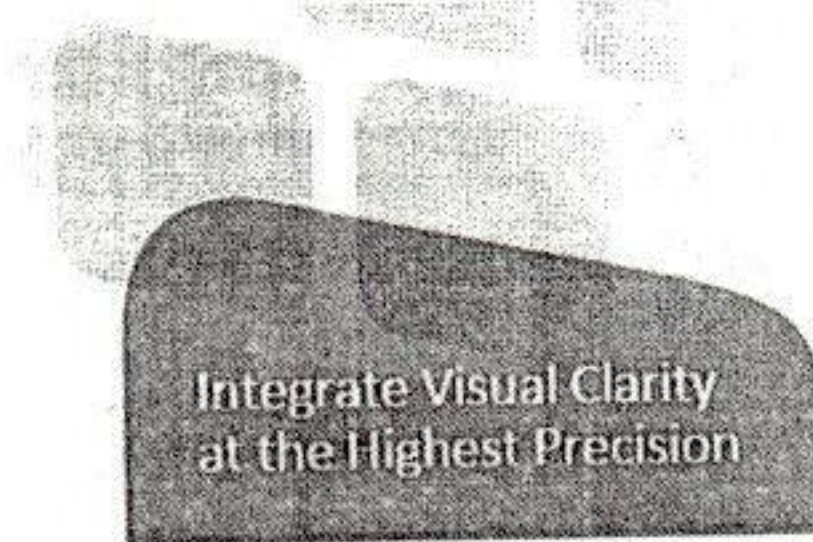


[Home](#) > [Products](#) > [Surgical Light](#)

VIDA X Series

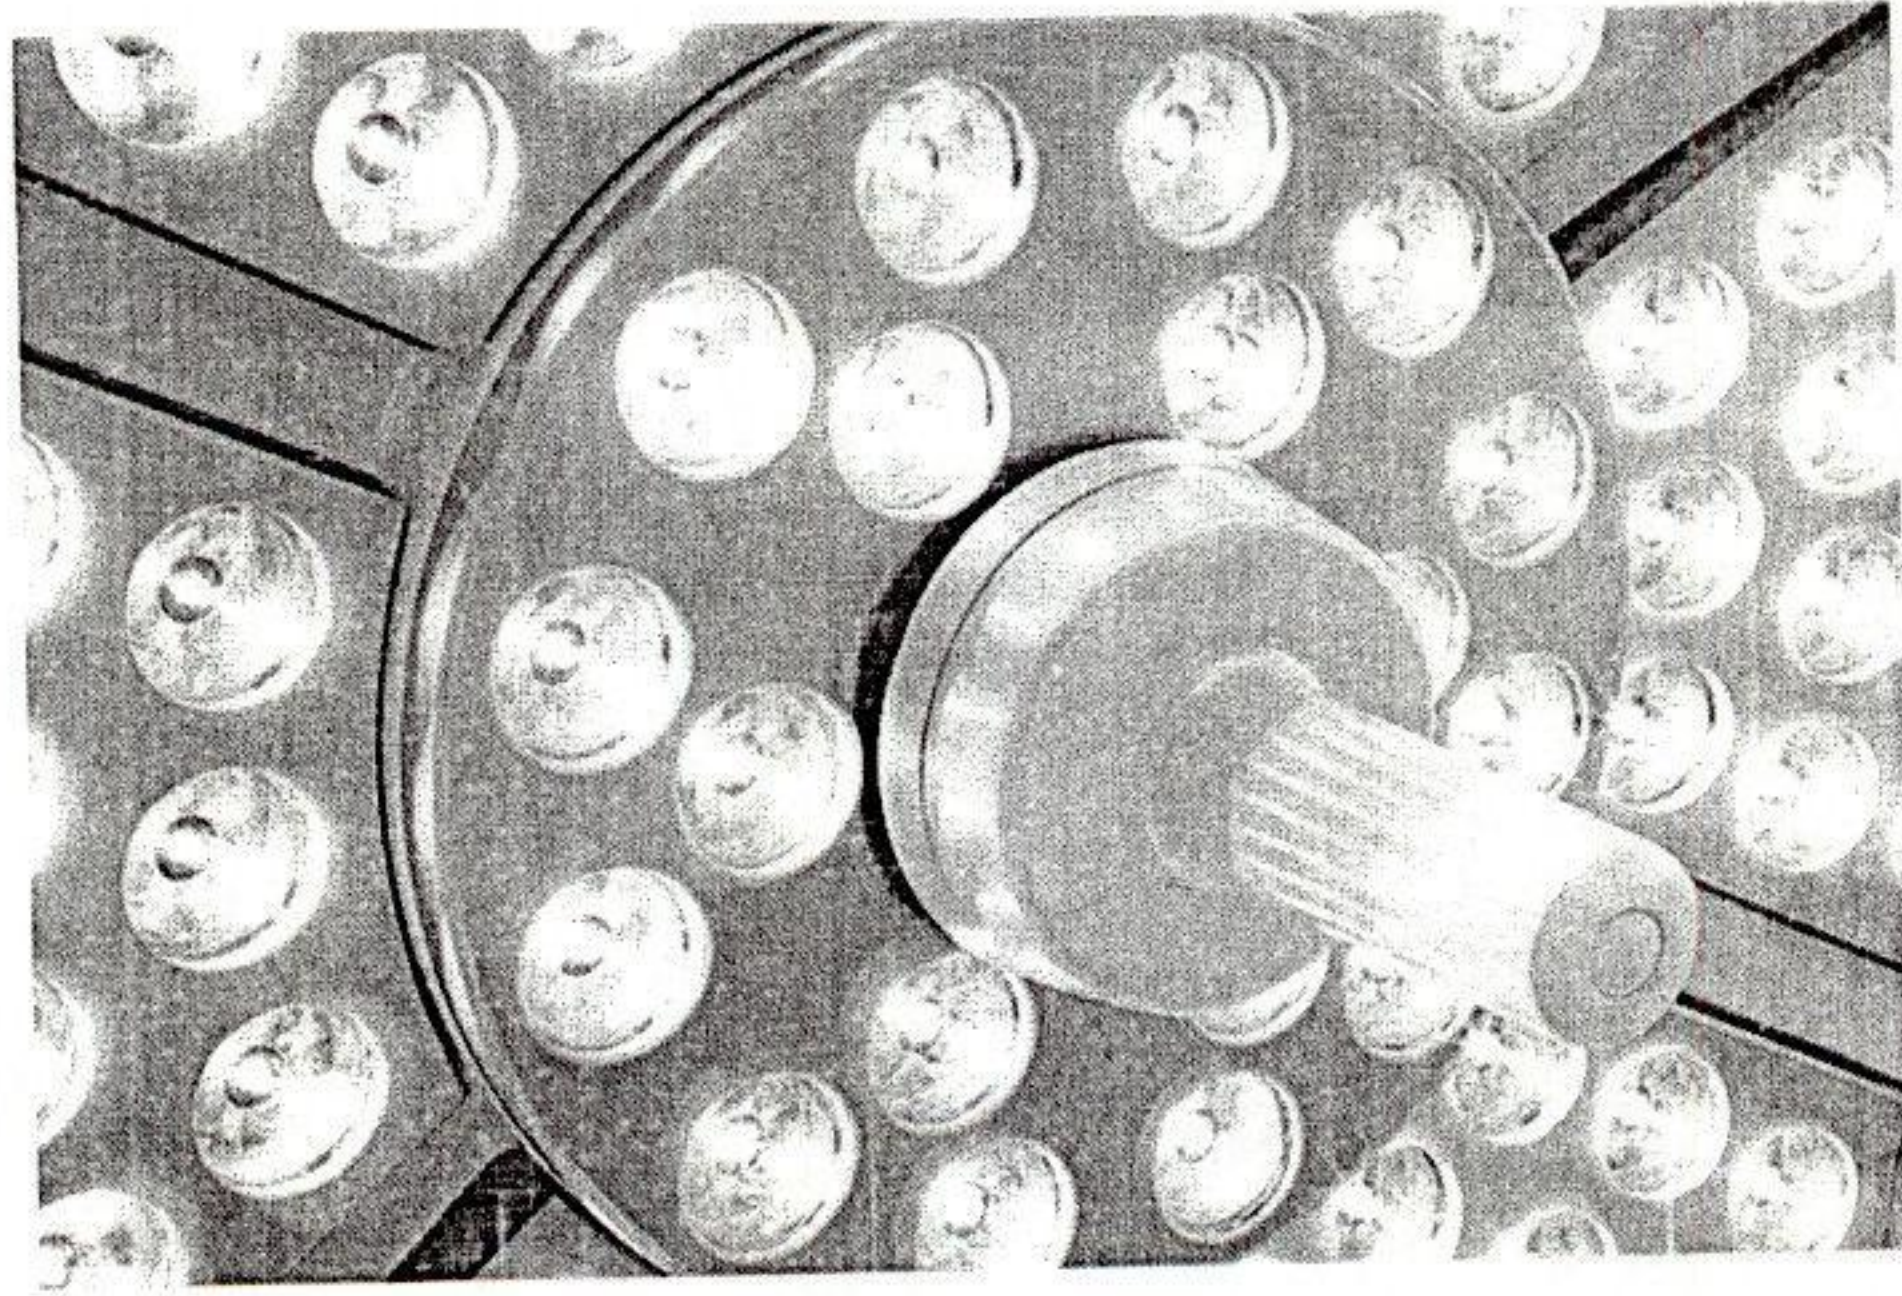


LED Advantages

- Cool and high-efficiency LEDs mean less heat on surgeon.
- Long lifetime with 5-year warranty on LEDs.
- Pure white light at 4200 Kelvins.
- High-intensity output at maximum 160,000 lux.

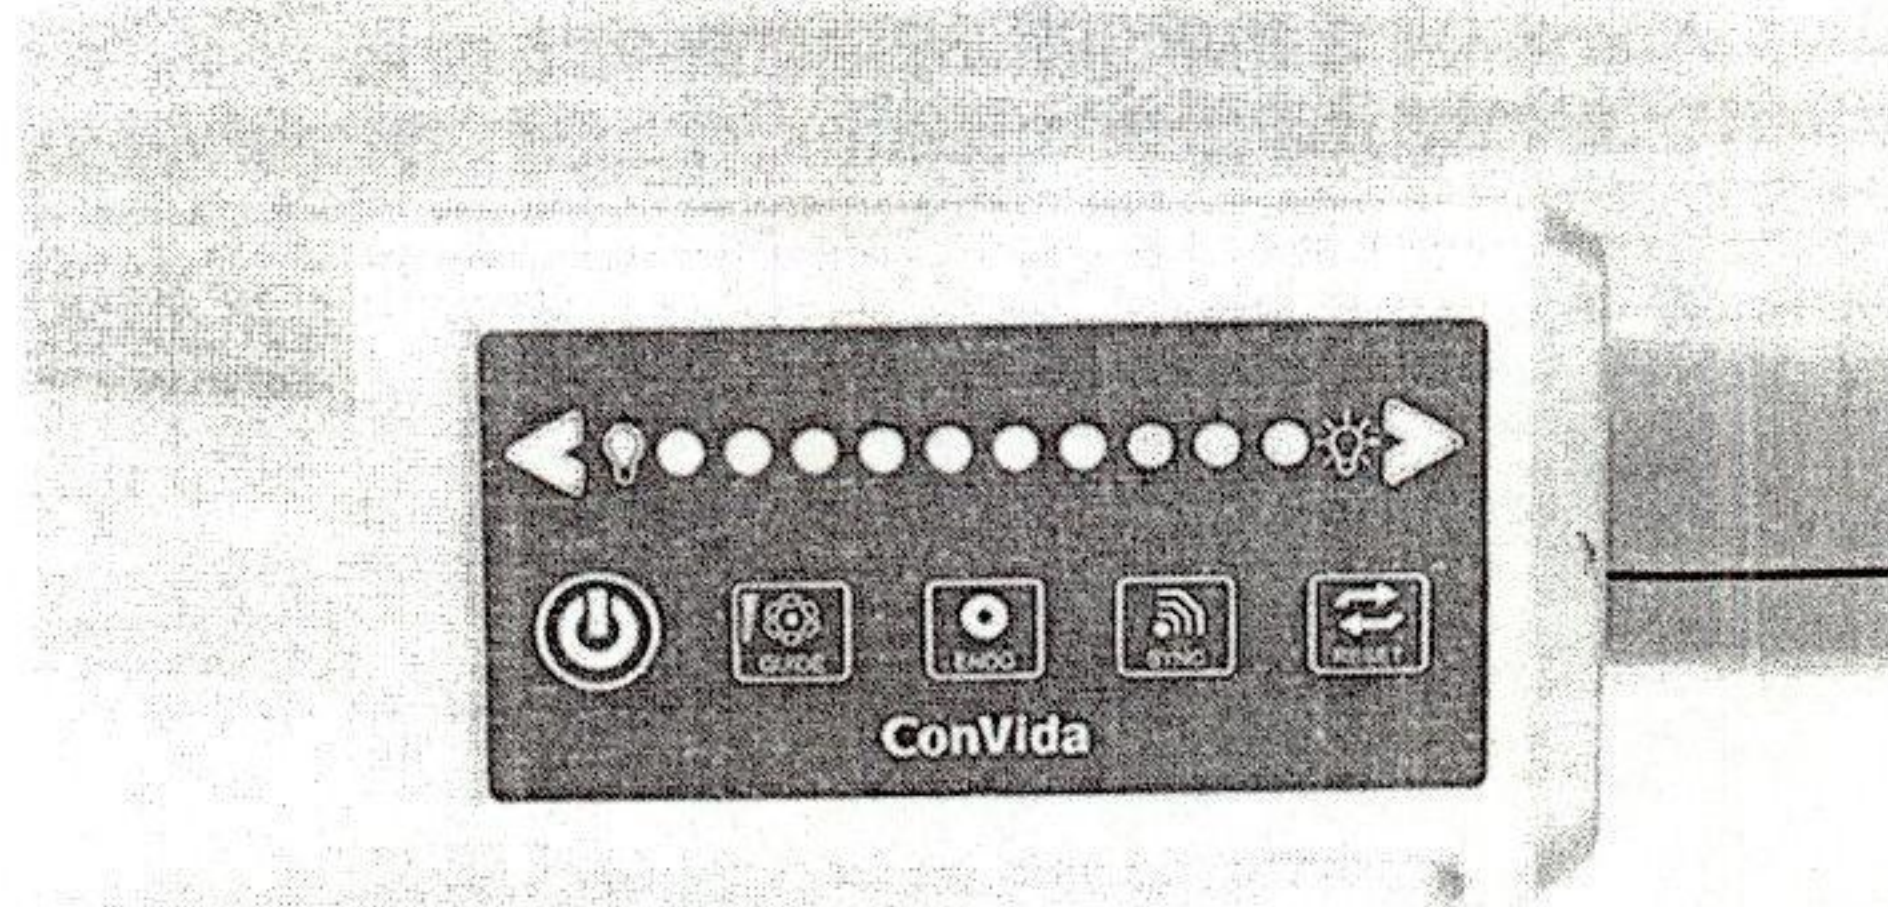


**Controls from
Lighthead and Wall**

- Intensity is controlled through slider bar or touch keypad.
- Synchronization of all lighting functions by activating SYNC button.

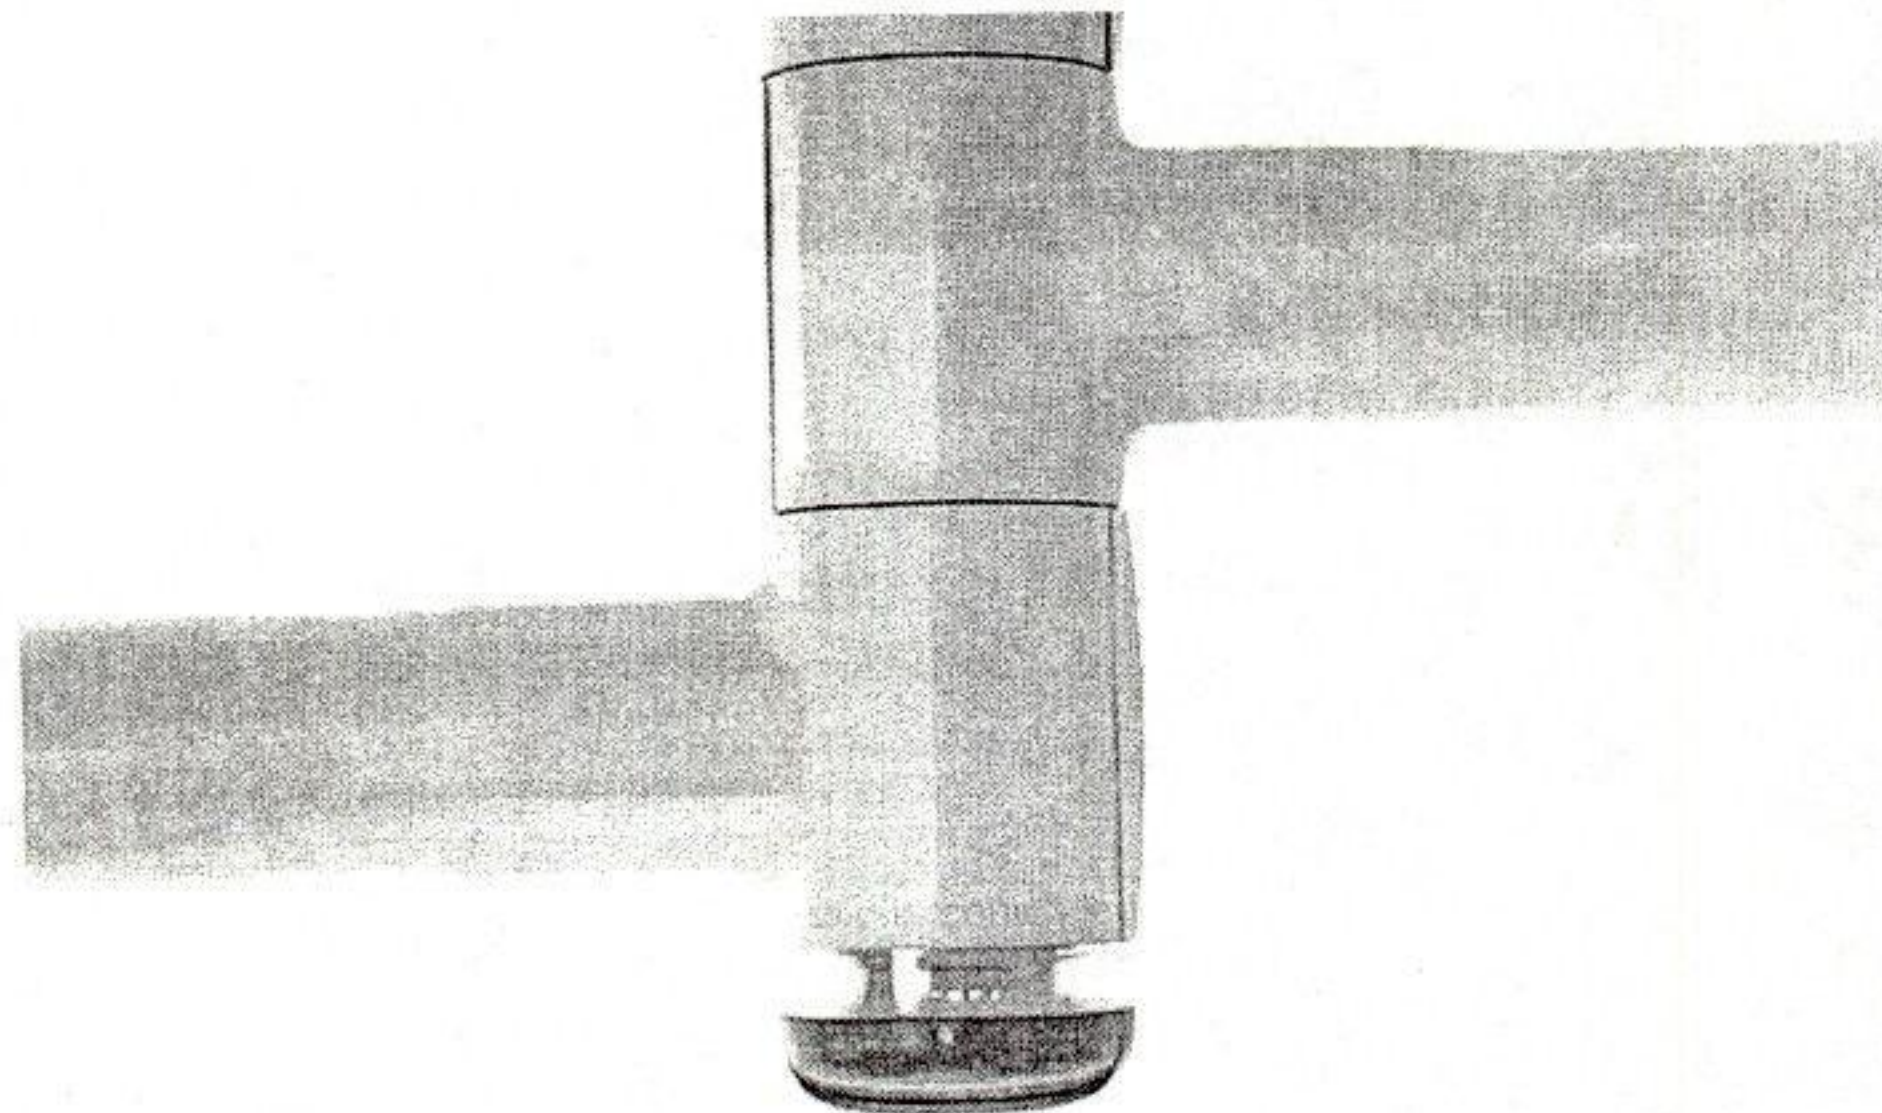

Two Ambient Lights




- Green ambient light (ENDO mode) sheds low-level green light.
- White ambient light (GUIDE mode) illuminates those LEDs at the center of the lighthead.

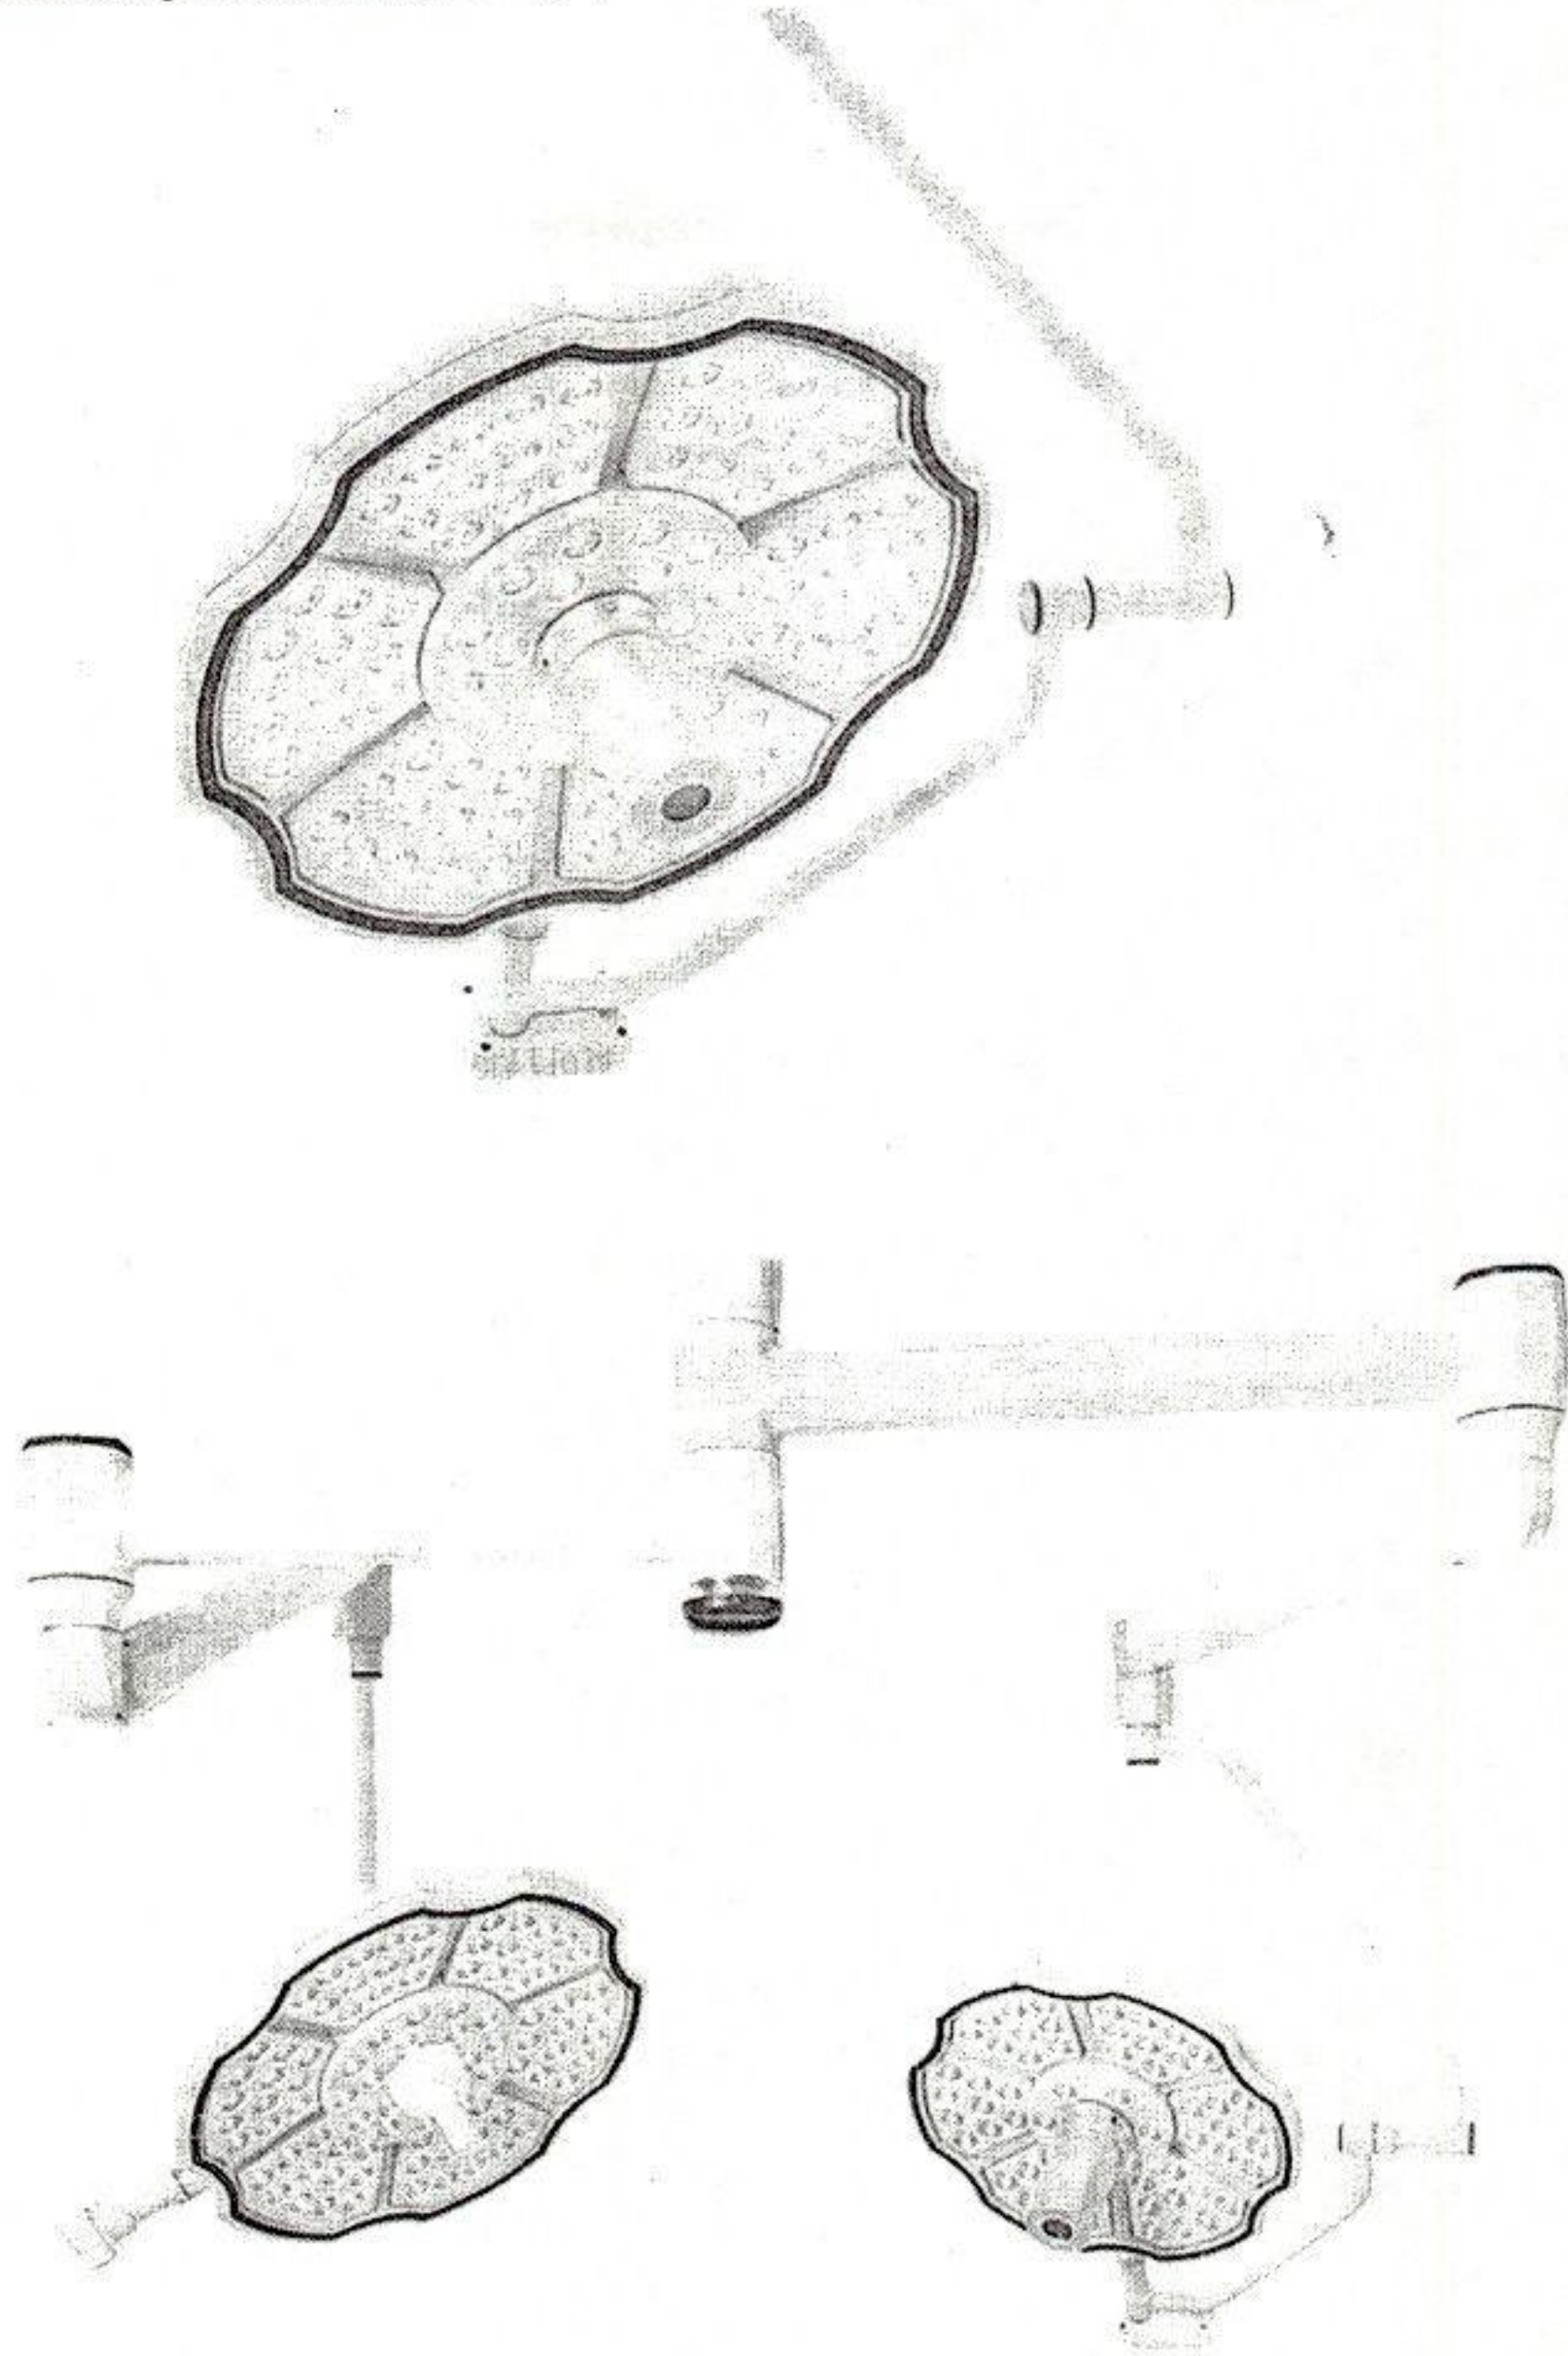

**Camera-Ready Lighthead
and Suspension**

- The lighting system is pre-wired for an optional plug-and-play VIDA HD camera.
- Advanced design in suspension supports HD video transmission while allowing 360° rotation on all key joints.

Mobile Unit - VIDA X50/R

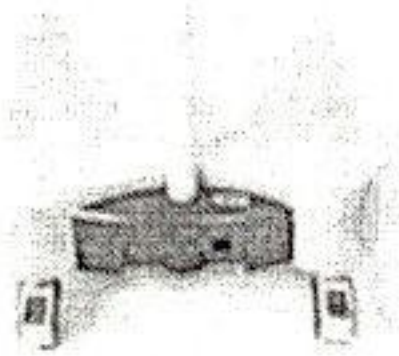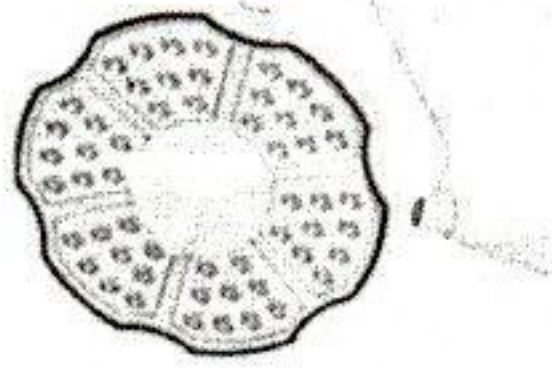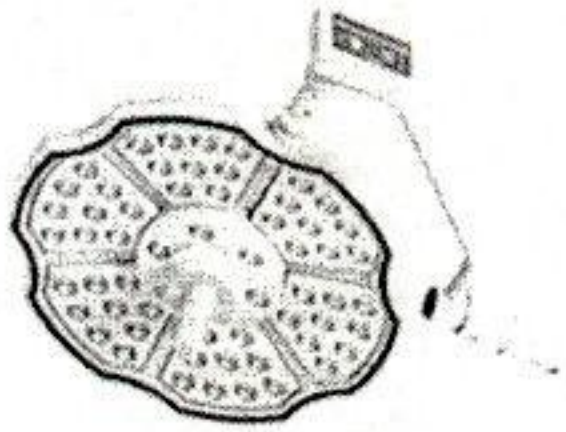

AMBIENT LIGHTING

- GUIDED lighting provides low level white illumination and can be configured through lighting control.

BACKLIGHT BATTERY INDICATOR

- The level of remaining power is clearly visible on the backlight battery indicator.

Features

LED Advantages

- Cool and high-efficiency LEDs mean less heat on surgeon.
- Long lifetime with 5-year warranty on LEDs.
- Pure white light at 4200 Kelvins.
- High-intensity output at maximum 160,000 lux.

Illumination and Long Depth

- Focus is adjustable through 157 cm beneath the lighthead.
- Reduced shadow gives optimal illumination in a deep cavity.
- Light intensity adjustable from 10%~100%.

Two Ambient Lights

- Green ambient light (ENDO mode) sheds low-level green light.
- White ambient light (GUIDE mode) illuminates those LEDs at the center of the lighthead.

Controls from Lighthead and Wall

- Intensity is controlled through slider bar or touch keypad.
- Synchronization of all lighting functions by activating SYNC button.

Camera-Ready Lighthead and Suspension

- The lighting system is pre-wired for an optional plug-and-play VIDA HD camera.
- Advanced design in suspension supports HD video transmission while allowing 360° rotation on all key joints.

Specifications

Lighthead Data	X70	X50
Diameter of lighthead (cm)	72	58
Light source	LED	LED
Number Of LEDs	90	60
Average LED Life (hours)	50,000	50,000
Color temperature, Kelvins	4200	4200
illumination at 1m (lux)	160,000	130,000
illumination adjustment	10%~100%	10%~100%
Color rendering index, CRI	95	95
Red color index, R9	95	95
Light field size, D10 (cm)	20~32	18~28
D50/D10 (%)	> 50	> 50
Depth Of light L1+L2 20%	157	145
Remaining illumination (cm, one mask)	68%	60%
Remaining illumination (cm, two mask)	48%	47%
Remaining illumination (cm, w/ tube)	86.7%	96.7%
Remaining illumination (cm, one mask w/ tube)	53%	55%
Remaining illumination (cm, two mask w/ tube)	40%	45%
Power consumption	100W @24Vdc	80W @24Vdc

*The lighting data above described are subject to a tolerance of 10%.

Company Overview

Corporate Development

Philosophy of Business

Surgical Light

Examination Light

Suspension System

Video Solutions

and R&D

Regulatory / QA

Service

Technical Support

Career

info@convidahealthcare.com

3200 NW 37th Ave, Building 3, Suite 150
USA

Taiwan

TEL: +886-2-217-4999

info@convidahealthcare.com

No.33, Dinghu Rd., Gushan Township
33378, Taiwan

[Company Overview](#)

[Corporate Development](#)

[Philosophy of Business](#)

[Surgical Light](#)

[Examination Light](#)

[Suspension System](#)

[Video Solutions](#)

[and R&D](#)

[Regulatory / QA](#)

[Service](#)

[Technical Support](#)

[Career](#)

info@convidahealthcare.com

3200 NW 37th Ave. Building 3 Suite 1000
USA

Taiwan

7F, 333-8, Taiwan

info@convidahealthcare.com

No.33, Dinghu Rd., Guoshan Taichung
33378, Taiwan

MINUTES OF THE PROCUREMENT COMMITTEE FOR SMBB TRAUMA CENTRE

Meeting of the Procurement Committee of Trauma Centre - Civil Hospital Karachi was held on Friday 12-2013 at 11:00 a.m. in the Board Room. Prof. M. Saeed Quraishy, Medical Superintendent - Civil Hospital Karachi chaired the meeting. The financial bids were opened after finalization of technical bids by the Procurement Committee for procurement of Machinery / Equipments under Tender for Supply, Installation, Testing, Commissioning and Maintenance (during maintenance periods of Medical Equipments for "Shaheed Mohtarma Benazir Bhutto, Accident, Emergency & Trauma Center and Ancillary Services Complex at Civil Hospital Karachi for financial year 2013-2014. The technical bids at tender enquiry number PD-Trauma Centre-CHK/011 (Rev) 2013-14 were opened on 08-10-2013 and subsequently approved by the Procurement Committee for procurement of the required items. The committee decided that the number of items to be procured will vary as per requirements of respective departments of Civil Hospital Karachi which is also in line with Tender Condition.

The following members attended the meeting:

01	Prof. (Dr.) M. Saeed Quraishy Medical Superintendent, Civil Hospital Karachi	Chairperson
02	Prof. (Dr.) Khalida Soomro Chairman Department of Cardiology, Dow University of Health Sciences	Member
03	Prof. (Dr.) Sadqa Aftab Chairman Department of Anaesthesia, Dow University of Health Sciences	Member
04	Prof. (Dr.) Junaid Ashraf Chairman Department of Neurosurgery, Dow University of Health Sciences	Member
05	Engr. Hayat Kemal Project Director	Member
06	Mrs. Shaista Mubarak Addl. Director (Development), Health Department, Govt. of Sindh	Secretary Member
07	Dr. Abdul Jabbar Memon Deputy Director (Development), Health Department, Govt. of Sindh	Member
08	Mr. Saleem Ahmed Siddiqui Divisional Accounts Officer, A.G. Sindh Office	Member
09	Mr. Shahid Ali Khan Accounts Officer, Civil Hospital Karachi	Member

Initiating the discussions, this office presented the evaluated Technical Data Sheets for perusal of the Procurement Committee and subsequently the Financial Bids were opened as under:

Tender Enquiry No : PD-Trauma Centre-CHK/011 (Rev) 2013-14
 Item No. : 1
 Name of Item : Operation Theatre Light LED
 Quantity Required : 10 Units
 Estimated Price : Rs. 2,500,000/- each

Name of Firms	M/S Universal Enterprise	M/S Radiant Medical (Pvt.) Ltd.	M/S Noor International	M/S Sippex Hospital Supplies	M/S Sippex Hospital Supplies (Alternate Offer)	M/S Med Elec Corporation
Make	Brandon Medical	Trumpf	Siemon & Co. KG Medical GMBH	Convida	Convida	
Model	Modular Galaxt HD LLED5040	iLED5/iLED 3	Sim LED 7000/LH Sim LED 7000	Modular Convida LED OT Light Double Dome System X70	Modular Convida LED OT Light Double Dome System X50	

The offers of M/S Noor International, M/S Sippex Hospital Supplies (Alternate Offer) and M/S Med Elec Corporation were not considered by the Procurement Committee as the offered models were not according to the required specifications as per tender requisite.

The offers of M/S Radiant Medical, M/S Universal Enterprises and M/S Sippex Hospital Supplies and X-70 meet all the required specification as per tender requisite. As approved by the Procurement Committee, the financial offers of said firms were opened.

M/S Radiant offered the rates for Euro 27450/- each equivalent to Pak. Rs. 4,050,072 - each on CIF basis and PKR 4,776,470/- on DDP basis.

M/S Universal Enterprises offered the rate of GBP 21880/- each equivalent to Pak. Rs. 3,885,162/- each on CIF basis and PKR 3,739,000/- each on DDP basis. The offer for optional Modular camera system with medical grade monitor was GBP 25,300/- equivalent to Pak Rs. 4,492,440/- each on CIF basis and PKR 4,320,500/- on DDP basis.

M/S Sippex Hospital Supplies offered the rate of USD 23,275 each equivalent to Pak. Rs. 2,520,000/- each on CIF basis and PKR 2,500,000 on DDP basis. The offer for optional HD camera Handle Module with camera control unit was USD 17,300/- each equivalent to Pak. Rs. 1,877,808/- on CIF and PKR 1,862,000/- on DDP basis.

After opening of Financial Bids, M/S Radiant Medical (Pvt.) Ltd. requested for re-evaluation vide letter dated 16-12-2013 of this item (Copy enclosed). So a meeting was held in the office of Prof. Junaid Ashraf on 21-12-2013 and the technical bids of M/S Radiant Medical (Pvt.) Ltd. and M/S Sippex Hospital Supplies were re-evaluated thoroughly. As a result of that meeting Prof. Junaid Ashraf issued a letter to Project Director (Copy enclosed) for enquiring from M/S Radiant Medical (Pvt.) Ltd. to pin point deficiency in the Technical Bids of M/S Sippex Hospital Supplies. The letter was sent to M/S Radiant Medical (Pvt.) Ltd., who again represented vide letter No. 2812/13 dated 28-12-2013 (Copy enclosed). M/S Radiant Medical (Pvt.) Ltd. replied that letter and copy was sent to Medical Superintendent - Civil Hospital Karachi who forwarded that letter to Prof. (Dr.) Junaid Ashraf.

To have a second opinion on the matter a letter was written to M/S Naqvi & Siddiqui Associates (Consultants) vide No. PD/AEC&ASC/CIHK/2013/2749 dated 08-01-2014 regarding compatibility of O.T. Light with Laminar Flow. They were of the opinion that "No compatibility is required between Air Laminar and O.T - Light". So representation of M/S Radiant Medical (Pvt.) Ltd. was not accepted.

Handwritten signatures and initials at the bottom of the page, including "PP", "A", "D", "for April", and "21".

Subsequently this matter of compatibility was also discussed with M/S Captive Aire, who may install "Luminar Flow". They are also of the opinion that there is no issue of "Compatibility" (Copy enclosed).

The procurement Committee approved and accepted the offer of M/S Sippex Hospital Supplies at the rate of Rs. 2,526,357/- each on CIF basis.

Tender Enquiry No. : PD-Trauma Centre-CHK/011 (Rev) 2013-14
 Item No. : 2
 Name of Item : Blood Warmer with Accessories
 Quantity Required : 09 Units
 Estimated Price : Rs. 503,124/- each

Name of Firms	M/S Radiant Medical (Pvt.) Ltd.	M/S BIOS
Make	Barkey	Geratherm
Model	S-Line	BIO204

The offer of M/S Radiant Medical (Pvt.) Ltd. was not considered by the Procurement Committee as the offered model was not according to the required specifications as per tender requisite.

The offer of M/S BIOS meets all the required specification as per tender requisite. As approved by the Procurement Committee, the financial offer of said firm was opened.

M/S BIOS offered the rates for Euro 3410/- each equivalent to Pak. Rs. 503,124/- each on CIF basis and PKR 595,000/- on DDP basis.

The procurement Committee approved and accepted the offer of M/S BIOS at the rate of Rs. 503,124/- each on CIF basis.

Tender Enquiry No. : PD-Trauma Centre-CHK/011 (Rev) 2013-14
 Item No. : 3
 Name of Item : Infusion Warming System
 Quantity Required : 10 Units
 Estimated Price : Rs. 350,000/- each

Name of Firms	M/S BIOS	M/S Noor International
Make	Geratherm	The Surgical Co. International
Model	BIW 306	Fluido Blood & Fluido Warming System

The offer of M/S BIOS was not considered by the Procurement Committee as the offered model was not according to the required specifications as per tender requisite.

Handwritten signatures and initials are present at the bottom of the page, including "PD" and "31".

SUPPLY, INSTALLATION, TESTING, COMMISSIONING, AND MAINTENANCE (DURING MAINTENANCE PERIOD) OF MEDICAL EQUIPMENTS FOR THE PROJECT "SHAIKH MOHTARMA BENAZIR BHL (TO ACCIDENT, EMERGENCY AND TRAUMA CENTRE AND AUXILIARY SERVICES COMPLEX) AT CIVIL HOSPITAL KARACHI

TENDER NO. PD-TRAUMA CENTRE-CHK/011 (REV) 2013-14
 DATE OF OPENING: 13-12-2013 (FINANCIAL PROPOSALS)

Item No. 1
 Name of Item Operating Theatre Light LED
 Qty. 10

S.No.	Name of Qualified Firm	CIF Price		Quoted Amount		Earnest Money
		Unit Price	Total Price	Unit Price	Total Price	
1	M/S Radiant Medical	Euro 27450	Euro 274500	PKR 4776470	PKR 47764700	CDRSDM 06/2641 (d. 04-10-2013) Bank Al-Falah Ltd. (0044) Sheadan, Lahore Rs. 950000/-
2	M/S Universal Enterprises	Pounds 21880	Pounds 218800	PKR 3739930	PKR 37399300	7487931 (d. 07-10-2013) United Bank Ltd. (0150) Chaudhri Chowk, Karachi Rs. 2852000/-
OPTIONAL:						
	Module Camera System with Medical grade Monitor	Pounds 25300	Pounds 253000	PKR 4320500	PKR 43205000	
3	M/S Supras Hospital Supplies (New LED X-70)	USD 23275 Optional: USD 17300	USD 232750 Optional: USD 173000	PKR 2500000 Optional: 1862000	PKR 25000000 Optional: 18620000	7487931 (d. 07-10-2013) United Bank Ltd. (0150) Chaudhri Chowk, Karachi Rs. 893500/-
OPTIONAL:						
	HD Camera Handle Module	USD 7500	USD 75000	PKR 1862000	PKR 18620000	
	3.77 Mega Pixel with camera control unit	USD 7500	USD 75000	PKR 1862000	PKR 18620000	

(Handwritten signatures and initials)

(Large handwritten signature)

(Handwritten signature)

RADIANT MEDICAL (PVT) LTD.

A DYNAMIC FORCE IN PROGRESSIVE HEALTH CARE

16-12-2013

The Medical Superintendent
Civil Hospital Karachi
Karachi.

Sub: REQUEST FOR THE RE-EVALUATION OF MAIN OT LED LIGHT BID

Respected Sir,

With the reference of recent Tender of Civil Hospital Karachi Trauma Center, we would like to inform you that. we participated in this tender by name of Radiant Medical (Pvt) Ltd. and we would like to put your attention on item No.01 (Main OT LED Light) we quoted this item according to the tender generic specification, mention clearly in tender form but unfortunately, one company name, CIPEX or SIPEX quoted (CONVIDA Brand) which technical specification does not meet or even unmatchable with the tender published specification and kindly take action how it is technically qualify and reached till financial bid opening.

So, we hereby request you to please look in to this issue, seriously. Therefore, you are requested that please re-evaluate its Bid on Technical basis.

We are looking for your immediate response on this issue and we will be very grateful to you in this regard.

For Radiant Medical (Pvt) Ltd.

Technical Department



2015

PD

17/12/13

Person see
end use
17/12/2013
PD.



**OFFICE OF THE PROJECT DIRECTOR
SHAHEED MOHTARMA BENAZIR BHUTTO
Accident, Emergency & Trauma Centre and Ancillary
Services Complex at Civil Hospital Karachi**

NO: PD/AEC&ASC/CHK/2013/2697


DATED: DECEMBER, 26-2013

M/S Radiant Medical (Pvt.) Ltd.

**SUBJECT: REQUEST FOR THE RE-EVALUATION OF MAIN OT - LIGHT
BID**

- This refers to your representation on above subject.
- The same was sent to Mr. Junaid Ashraf / Prof. of Neurosurger for comments.
- He has replied as per the letter enclosed, please reply to the queries to the undersigned.

Copy to Medical Superintendent,
Civil Hospital Karachi


PROJECT DIRECTOR

Department of Neurosurgery
DOW MEDICAL COLLEGE & CIVIL HOSPITAL
KARACHI - PAKISTAN.



JUNAID ASHRAF
F.R.C.S. (Neurosurgery)
PROFESSOR OF
NEUROSURGERY

Tel. : 9215740
Ext. : 2512

Dated: 21st Dec, 2013

The Project Director,
Shaheed Mohtarma Benazir Bhutto,
Accident, Emergency & Trauma Centre and
Ancillary Services Complex at
Civil Hospital Karachi

SUBJECT: REQUEST FOR THE RE-EVALUATION OF MAIN OT - LIGHT BID

This is with reference to your above letter and the objection raised by M/S Radiant Medical (Pvt.) Ltd. regarding the OT Light of M/S SIPPEX (Modular CONVIDA LED OT Light Double Dome System X-70). The specification provided by M/S Sippex and two others are more or less similar, apart from minor differences. M/S Radiant Medical (Pvt.) Ltd should be asked to specify exactly as to what technical specifications is CONVIDA light deficient in.

Prof. Junaid Ashraf
Head of Department,
Department of Neurosurgery,
Dow University of Health Sciences

Sippex

HOSPITAL

D-169 Block-7
Gulshan-e-Iqbal
Karachi-Pakistan
Phone: +92-21-34930707
Fax: +92-21-34923878
Email: sippex-hs@cyber.net.pk

To,
The Project Director,
Shaheed Mohtarma Benazir Bhutto,
Accident, Emergency and Trauma Centre and Ancillary,
Services Complex at Civil Hospital,
Karachi.


Dated: 03-01-2014
Ref No.:004/SPX/CHK

Subject: CLARIFICATION FOR LAMINAR FLOW

- With Reference to your Letter No. PD/AFC&ASC/CHK/2014/2714, We M/S Sippex Hospital Supplies had already submitted the letter from principal regarding to clarification for Laminar Flow.
- Copy of clarification letter from the principal is attached with this letter

Please feel free to contact in case any further clarification is required.

Sincerely Yours,

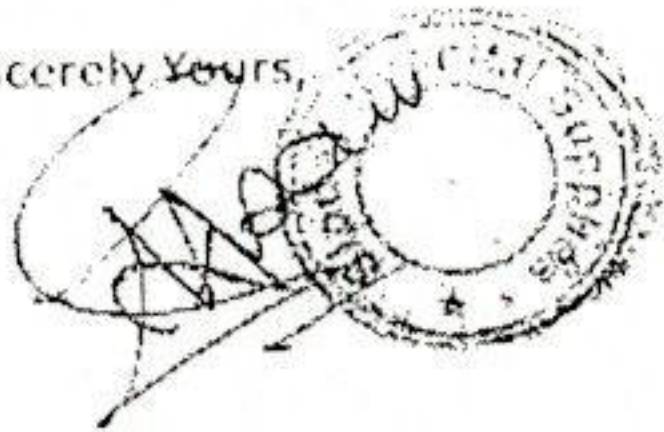

Sippex Hospital Supplies
Rasheedul Hassan
National Sales Manager
Ph: +92(0) 300 2269 015
Email: rasheedulhassan@live.com

Civil Hospital, Karachi
Pakistan

Sub: Technical Clarification

Ref. Your Tender Bid at Shahhed Mohatarnna Benazair Bhutto Accident, Emergency &
Trauma Center and Ancillary Services Complex.

Our offer for ConVida Brand VIDA LED Surgical Lighting System

Dear Sir/ Madam,

With reference to the above, please find below our point wise reply to the technical queries:

1. A modular OT light which should deliver optimal lighting quality with highest degree adaptability and energy efficient LED light:
 - Our lights are modular designed with various available configurations. The lighting performance will help shadow-less surgical operation.

2. Be compatible with laminar flow system:
 - Our lighthead is compact with obstructed surfaces of 4800 cm² which is as small as most LED brands biggest lighthead in the market. Therefore, our O.T. lamp will not give much impact of the laminar flow.


Hope above clarifies. Please feel free to revert in case any further clarification is required.

Sincerely yours,



ConVida Healthcare & Systems
Evelyn H. Ning
Sales/Marketing Director



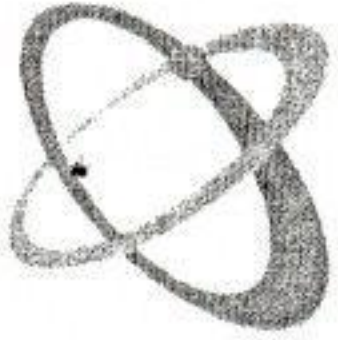

RADIANT MEDICAL (PVT) LTD.

A DYNAMIC FORCE IN PROGRESSIVE HEALTH CARE

Doc Ref No: 2814/13
Date: 28.12.2013

*Received
28/12/13*

The Project Director
Shaheed Mohtrama Benazeer Bhutto
Accident, Emergency & Trauma Center And
Ancillary Services Complex At
Civil Hospital Karachi

Subject: REQUEST FOR THE RE-EVALUATION OF MAIN OT-LIGHT BID

Respected Sir,

With the reference of your letter Number PD/AEC&ASC/CHK/2013/2697, dated 26.12.2013 regarding above mention subject and as per your Technical comparison between Trumpf LED LIGHT-Germany & ConVida-Taiwan, OT Light. In which Dr. Junaid Ashraf professor of neurosurgery mentioned his 21st December 2013 letter, and asking specification deficient of ConVida (Attached copy of letter). He said there is minor difference between these two light but sorry to say we can't agree with his point of view, because a surgeon can't compromise with the light, following are the major deficiency against published Specification

- Less Intensity / Lux
- Fix Focus
- No Compatibility with the Laminar Air Flow
- No Shadow Management/control
- Less CRI
- Fix Color Temperature
- Taiwan is not equivalent to USA, EEC, Japan

And on the basis of above specification which are not match with the required tender published specification, it cannot be technically qualify, therefore you are requested please take this matter seriously and take decision accordingly.

We are looking for your immediate response on this issue and we will be very grateful in regard to this regards

For Radiant Medical (Pvt.) Ltd.

Technical Departments

- CC to Medical Superintendent Civil Hospital Karachi
- CC to Head of Department Neurosurgery CHHS

Technical Comparing Between Trumpf Germany & ConVida Taiwan

Parameter	Trumpf Germany	ConVida Taiwan
Laminar Air Flow Compatible	YES	No (Not Possible)
Shadow Controlled	Yes available	No (Not Possible)
Light Intensity	320,000lux	290,000 Lux
Colour Rendering Index (CRI)	98	95
Colour Temperature	3,500-4,000-4,500-5,000 K	4,200 Fixed
Auto Focus	Yes, Auto Focus	No, Fixed Focus (Not available)

Blumenthal
 29/11/2012
 Peter N. G. ...
 PD

2013
 PD
 2012.5


Products

- O.R. Integration
- Surgical Light
- VIDA X Series
- VIDA V Series (New)
- Examination Light
- Suspension System
- Video Solutions


Surgical Light

Integrate Visual Clarity
at the Highest Precision

[Home](#) > [Products](#) > [Surgical light](#)


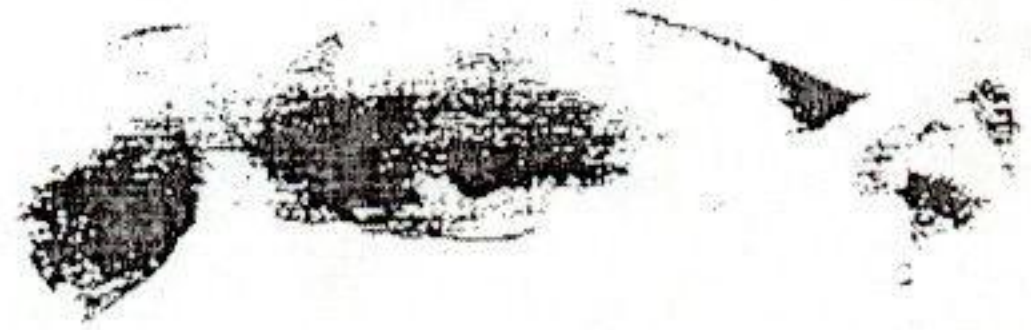


VIDA X Series

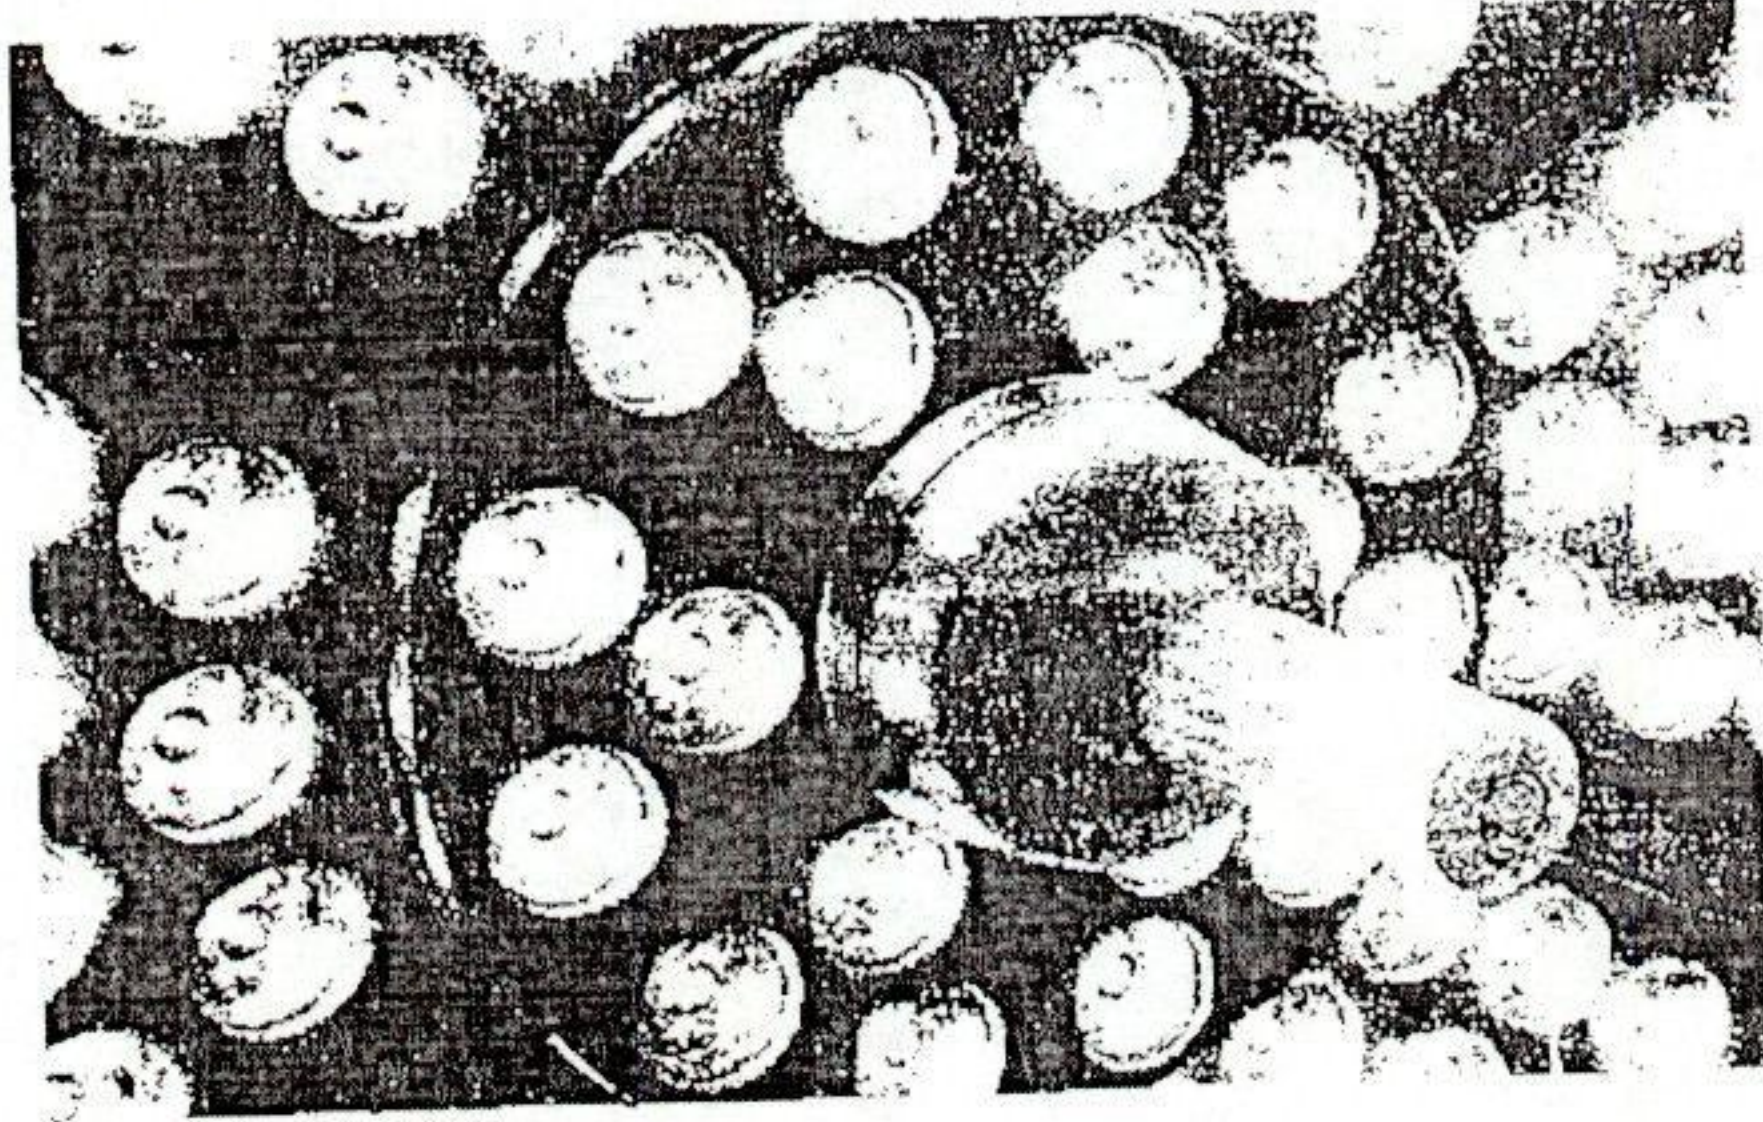

LED Advantages

- Cool and high-efficiency LEDs mean less heat on surgeon.
- Long lifetime with 5-year warranty on LEDs.
- Pure white light at 4200 Kelvins.
- High-intensity output at maximum 160,000 lux.

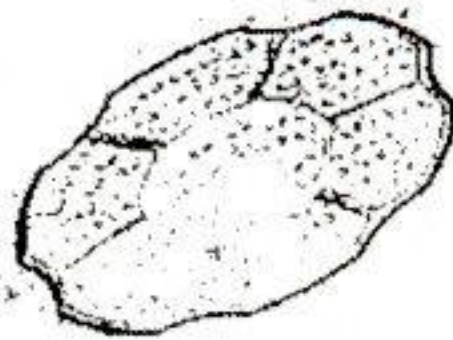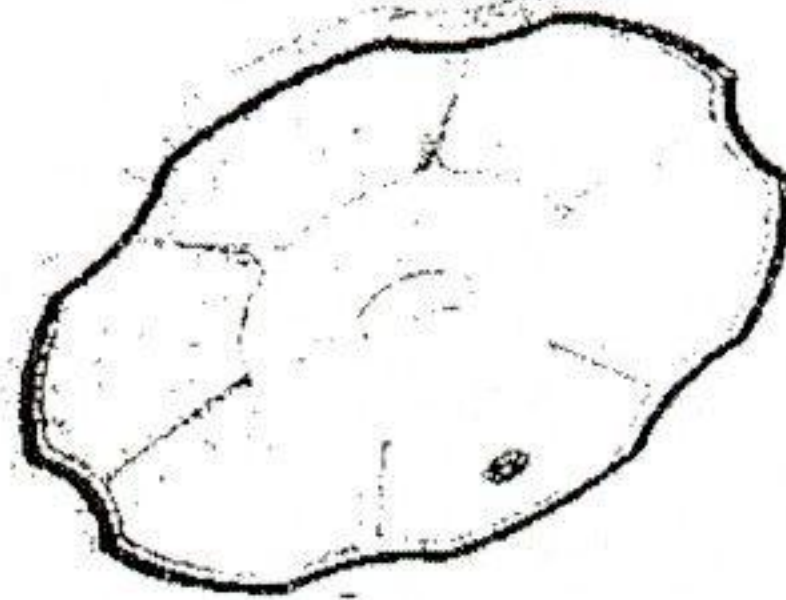

**Camera-Ready Lighthead
and Suspension**

- The lighting system is pre-wired for an optional plug-and-play VIDA HD camera.
- Advanced design in suspension supports HD video transmission while allowing 360° rotation on all key joints.

Mobile Unit - VIDA X50/R



AMBIENT LIGHTING

- GUIDED lighting provides low level white illumination and can be controlled through lighting control.

BACKLIGHT BATTERY INDICATOR

- The level of remaining power is clearly visible on the backlight battery indicator.

Features

LED Advantages

- Cool and high-efficiency LEDs mean less heat on surgeon.
- Long lifetime with 5-year warranty on LEDs.
- Pure white light at 4200 Kelvins.
- High-intensity output at maximum 160,000 lux.

Illumination and Long Depth

- Focus is adjustable through 157 cm beneath the lighthead.
- Reduced shadow gives optimal illumination in a deep cavity.
- Light intensity adjustable from 10%~100%.

Two Ambient Lights

- Green ambient light (ENDO mode) sheds low-level green light.
- White ambient light (GUIDE mode) illuminates those LEDs at the center of the lighthead.

Controls from Lighthead and Wall

- Intensity is controlled through slider bar or touch keypad.
- Synchronization of all lighting functions by activating SYNC button

Camera-Ready Lighthead and Suspension

- The lighting system is pre-wired for an optional plug-and-play VIDA HD camera.
- Advanced design in suspension supports HD video transmission while allowing 360° rotation on all key joints.

Specifications

Lighthead Data	X70	X50
Diameter of lighthead (cm)	72	58
Light source	LED	LED
Number Of LEDs	90	60
Average LED Life (hours)	50,000	50,000
Color temperature, Kelvins	4200	4200
Illumination at 1m (lux)	160,000	130,000
illumination adjustment	10%~100%	10%~100%
Color rendering Index, CRI	95	95
Red color index, R9	95	95
Light field size, D10 (cm)	20~32	16~28
D50/D10 (%)	> 50	> 50
Depth Of light L1+L2 20%	157	145
Remaining illumination (cm, one mask)	68%	60%
Remaining illumination (cm, two mask)	48%	42%
Remaining illumination (cm, w/ tube)	86.7%	96.7%
Remaining illumination (cm, one mask w/ tube)	53%	55%
Remaining illumination (cm, two mask w/ tube)	40%	45%
Power consumption	100W @24Vdc	80W @24Vdc

*The lighting data above described are subject to a tolerance of ±2%

About
History

Products
O.R. Integration

Solution
Product Engineering

Contact
Customer

U.S.A.

Convida Systems Inc., O.R. Integration, LED Surgical Light, Surgical Light, LED Examination Light, Examination Light, Suspension System, Video Solutions

Company Overview

Surgical Light

and R&D

Service

Corporate Development

Examination Light

Regulatory / QA

Technical Support

Philosophy of Business

Suspension System

Career

Taiwan

Video Solutions



**OFFICE OF THE PROJECT DIRECTOR
SHAHEED MOHTARMA BENAZIR BHUTTO
Accident, Emergency & Trauma Centre and Ancillary
Services Complex at Civil Hospital Karachi**

NO: PD/AEC&ASC/CHK/2013/2749

DATED: JANUARY, 08-2014

M/S Naqvi & Siddiqui Associates (Consultants),
Karachi

SUBJECT: SUPPLY, INSTALLATION, TESTING, COMMISSIONING & MAINTENANCE (DURING MAINTENANCE PERIOD) OF MEDICAL EQUIPMENTS FOR THE PROJECT SHAHEED MOHTARMA BENAZIR BHUTTO ACCIDENT, EMERGENCY & TRAUMA CENTRE AND ANCILLARY SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI

- The above item was tendered by the office of the undersigned and M/S Sippex Hospital Supplies have offered OT Light of brand "CONVIDA - USA".
- A competitor has objected that this OT - light that it is not compatible to the Laminar Flow.
- Kindly advise in this matter whether this will affect the performance of Operation Theatre over all?
- A letter of M/S CONVIDA HEALTHCARE & SYSTEMS is also enclosed.

MIA (info for 200)
Pr excami & advice

P/D
an associate
Comments is

[Signature]
PROJECT DIRECTOR

Forwarded to NSA
28/01/14
No compatibility is required
between Air Laminar and O.T Light
M/S [Signature]
8-1-2014

Self explanatory

[Signature]

Print

<https://aa-mg5.mail.yahoo.com/m20/launch?revision=1379214347>

details please visit www.convidahealthcare.com.

Regards

IQTIDAR HUSSAIN



**OFFICE OF THE PROJECT DIRECTOR
SHAHEED MOHTARMA BENAZIR BHUTTO
Accident, Emergency & Trauma Centre and Ancillary
Services Complex at Civil Hospital Karachi**

NO: PD/AEC&ASC/CHK/2013/2665

DATED: DECEMBER, 11-2013

SUBJECT: TENDER FOR THE WORK "SUPPLY & INSTALLATION OF ALUMINUM CLADDING / CURTAIN WALL, SIGNAGE / MURALS & INTERNAL EXTERNAL ALLIED DEVELOPMENT WORKS" FOR THE PROJECT "SHAHEED MOHTARMA BENAIZIR BHUTTO ACCIDENT, EMERGENCY & TRAUMA CENTER AND ANCILLARY SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI"

TECHNICAL BID EVALUATION REPORT

- 1) The tenders for the above work were called through press and appeared in daily "Dawn" and "Ibrat" dated 23-09-2013 and on SPPRA Website with I.D. No. 1575213090 (Copy enclosed).
- 2) In response of above following Two prospective bidders purchased Tender Documents till closing date:-
 1. M/S INTERACT
 2. M/S ALCOP
- 3) The tenders were opened on 08-10-2013 in presence of the following Members of Procurement Committee alongwith representative of M/S Naqvi & Siddiqui Associates (Consultants):-
 1. Prof. M. Saeed Quraishy
Medical Superintendent – Civil Hospital Karachi / Chairman
 2. Prof. (Dr.) Khalida Soomro
Chairman – Department of Cardiology, Dow University of Health Sciences / Member
 3. Prof. (Dr.) Sadqa Aftab
Chairman – Department of Anaesthesia, Dow University of Health Sciences / Member
 4. Prof. (Dr.) Junaid Ashraf
Chairman – Department of Neurosurgery, Dow University of Health Sciences / Member
 5. Engr. Hayat Kemal
Project Director / Member
 6. Mrs. Shaista Mubarak
Additional Director (Development) Health Department – Govt. of Sindh / Member

7. Dr. Abdul Jabbar Memon
Deputy Director (Development) Health Department – Govt. of Sindh / Member
8. Mr. Saleem Ahmed Siddiqui
Divisional Accounts Officer – A.G. Sindh Office / Member
9. Mr. Shahid Ali Khan
Accounts Officer – Civil Hospital Karachi / Member

4) Following two participated in the opening and technical bids were opened:-

1. M/S INTERACT
2. M/S ALCOP

5) The Technical Bids were sent to M/S Naqvi & Siddiqui Associates (Consultants) for scrutinizing the same.


6) They have submitted the report and have technically qualified as under:-


1. M/S ALCOP **Recommended** for Prequalification as they have obtained 80% marks (more than fixed passing mark i.e. 75%).
2. M/S INTERACT **Not Recommended** for Prequalification as they have obtained 45% marks (less than fixed passing mark i.e. 75%).

7) A detail report of M/S Naqvi & Siddiqui Associates (Consultants) is also enclosed.



Medical Superintendent
Civil Hospital Karachi


Chairperson
Department of Cardiology

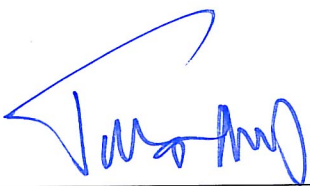
Chairperson
Department of Anaesthesia


Chairman
Department of Neurosurgery


Project Director


Addl. Director (Development),
Health Deptt: Govt. of Sindh


Deputy Director (Development),
Health Deptt: Govt. of Sindh


Divisional Accounts Officer
A.G. Sindh Office


Accounts Officer
Civil Hospital Karachi

SHAHEED MOHTARMA BENAZIR BHUTTO Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital, Karachi

TENDER NOTICE

Civil Hospital Karachi invites sealed bids on Single-Stage — Two-Envelope procedure as per Sindh Public Procurement Regulatory Authority Rules from the Manufacturers / Importers / Sole Agents / Contractors for the following works in Civil Hospital, Karachi.

S. No.	Name of Work	Bidding Document Cost (Rs.)	Earnest Money / Tender Security	Tender Purchasing Date or before	Date of Submission and Opening	Time of Completion of Works
1.	Supply, Installation of Aluminum Cladding / Curtain Wall Signage / Murals & Internal External Allied Development Works at "Shaheed Mohtarma Benazir Bhutto, Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital, Karachi"	1000/-	2% of Bid Amount	07-10-2013	08-10-2013 at 11:00 am and 08-10-2013 at 11:30 a.m. respectively	Three (3) Months

- A complete set of tender documents containing BOQ, Specification and Terms & Conditions can be purchased from the Office of the Project Director, Shaheed Mohtarma Benazir Bhutto Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital Karachi through Pay Order of Rs. 2000/- in favour of Project Director, Shaheed Mohtarma Benazir Bhutto Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital, Karachi on submission of application along with copy of NTN Certificate.
- The bid must be submitted on the respective dates by 11:00 a.m. in Board Room of the Administration Block of Civil Hospital, Karachi situated on second floor.
- These bids will be opened publicly at 11:30 a.m. on the same day in the presence of bidders or their authorized representatives who chose to attend on the place of submission.
- Technical and Financial proposals should be submitted in separate envelopes and both should be sealed in third envelope.
- All quotations shall include Government Taxes (if applicable) and these will be deducted from the bills, according to Government Rules.
- Bid Security @2% of total value of the quoted items by the firms in shape of Pay Order / Demand Draft must be attached with "Financial Bid" in favour of the Project Director, Shaheed Mohtarma Benazir Bhutto Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital, Karachi.
- In case of announcement of public holiday or any unfavourable circumstances, the tenders / bids will be opened on the next working day at the same time & venue.

INF-KRY: No. 2124

PROJECT DIRECTOR

23rd
MONDAY
DAILY
Dawn
23/9/2013
[Signature]

شهيد محترم بينظير ڀٽو
ايڪسيڊنٽ، ايمرجنسي ۽ ٽراما سينٽر ۽ اينڪلري
سروسز ڪامپليڪس آيت سول اسپتال ڪراچي

ٽينڊر نوٽيس

سول اسپتال ڪراچي پاران سنڱل اسٽيج - نو اٽويلب پروسيجر - سنڱ پبلڪ پروڪيورمينٽ ريگيوليٽري اٿارٽي رولز جي تحت مينوفڪچررز امپورٽرز سول اينجنٽس نيگيڊارن کان سول اسپتال ڪراچي جي هيٺ ڄاڻايل ڪمن جي لاءِ مھربند ٽينڊر ڪھرائي

نمبر	آئٽم	قيمت	سوٽي رقم	ٽينڊر خريد ڪرڻ جي تاريخ	جمع ڪرائڻ ۽ ڪولڻ جي تاريخ	علمو
1	شهيد محترم بينظير ڀٽو، ايڪسيڊنٽ، ايمرجنسي ۽ ٽراما سينٽر ۽ اينڪلري سروسز ڪامپليڪس آيت سول اسپتال ڪراچي ۾ اليوٽنر ڪلاوٽنگ ڪرڻين وال، اسٽيج ميورالز جي سيل، ليڪائن ۽ انٽروني گئزيل ترقياتي ڪمن جي ليڪائن	1080	اڇيل رقم جو 2 سيڪڙو	07.10.13	08.10.13 تي 11.00 وڳي ۽ 08.10.13 تي 11.30 وڳي ترميموار	3 مهينا

ٽينڊر جي ڪاغذن جو مڪمل سيٽ بي او ڪيو تي مشتمل شرطن ۽ ضابطن سميت آفيس آف ڊي پراجيڪٽ ڊائريڪٽر شهيد محترم بينظير ڀٽو ايڪسيڊنٽ، ايمرجنسي ۽ ٽراما سينٽر ۽ اينڪلري سروسز ڪامپليڪس آيت سول اسپتال ڪراچي وٽان 20000 روپين جي بي آرڊر عيوض پراجيڪٽ ڊائريڪٽر شهيد محترم بينظير ڀٽو ايڪسيڊنٽ، ايمرجنسي ۽ ٽراما سينٽر ۽ اينڪلري سروسز ڪامپليڪس آيت سول اسپتال ڪراچي جي حق ۾ تيار ٿيل درخواست ۽ اين تي اين جمع ڪرائڻ عيوض حاصل ڪري سگهجن ٿا. آڇ جا ڪاغذ ترميموار تاريخن تي 11.00 وڳي پورڊ روم آف اينجنٽس ريشن بلاڪ آف سول اسپتال ڪراچي واقع بي ماڙ تي جمع ڪيا ويندا.

اڇون سرعام 11.30 وڳي ان وقت تي موجود هجڻ جي خواهشمند آڇ ڏيندڙن جي موجودگي ۾ ڪوليون وينديون ٿيڪنيڪل ۽ فنانشل اڇون الڳ الڳ لفافن ۾ بند ڪري ٽئين لفافي ۾ مھربند ڪيون وڃن. سموريون اڇون حڪومت جي لاڳو ٿيندڙن ٿيڪسن تي مشتمل هجڻ جيڪي حڪومت جي قانون موجب ڪانجا ويندا.

ڪل اڇيل رقم جو 2 سيڪڙو فرم پاران بي آرڊر ڏيکارڻ جي وقت جي صورت ۾ لازمي طور فنانشل اڇن جي صورت ۾ پراجيڪٽ ڊائريڪٽر شهيد محترم بينظير ڀٽو ايڪسيڊنٽ، ايمرجنسي ۽ ٽراما سينٽر ۽ اينڪلري سروسز ڪامپليڪس آيت سول اسپتال ڪراچي جي حق ۾ تيار ٿيل جمع ڪرايو وڃي.

حڪومت پاران عام موڪل جو اعلان ٿيڻ يا ائٽر سببن جي ڪري ٽينڊر نه ڪلڻ جي صورت ۾ ساڳيون اڇون ٽينڊر ٻئي ڪم واري ڏينهن تي ساڳي وقت ۽ هنڌ تي ڪوليون وينديون.

پراجيڪٽ ڊائريڪٽر










17482	SPPRA ID WITHHELD	Khairpur Construction Work		30 Sep 2013	30.Sep.2013	23.Oct.2013	BER & CS Required
17481	SPPRA ID WITHHELD	1575213094 Executive Engineer Highway Division Dadu Construction of Roads		30 Sep 2013	30.Sep.2013	11.Oct.2013	BER & CS Required
17480	SPPRA ID WITHHELD	1575213093 Town Committee Khipro District Sanghar Construction of Roads		30 Sep 2013	29.Sep.2013	11.Oct.2013	BER & CS Required
17479	SPPRA ID WITHHELD	1575213092 Town Health Officer Liaquatabad Karachi Drugs/Medicines and Others		30 Sep 2013	29.Sep.2013	14.Oct.2013	BER & CS Required
17478	SPPRA ID WITHHELD	1575213091 Irrigation & Power Dept. Executive Engineer Jamrao Division Mirpurkhas Construction Work		30 Sep 2013	30.Sep.2013	15.Oct.2013	BER & CS Required
17477	SPPRA ID WITHHELD	1575213090 Shaheed Mohtarma Benazir Bhutto Accident, Emergency & Trauma Centre at Civil Hospital Karachi Miscellaneous Items		30 Sep 2013	22.Sep.2013	08.Oct.2013	BER & CS Required
17476	SPPRA ID WITHHELD	1575213089 Executive Engineer Provincial Coastal Highway Division Hyderabad Construction of Roads		30 Sep 2013	27.Sep.2013	22.Oct.2013	BER & CS Required
17475	SPPRA ID WITHHELD	1575213088 Executive Engineer Machinery Maintenance Division Digri @ Koldiji Construction of Roads		30 Sep 2013	30.Sep.2013	11.Oct.2013	BER & CS Required
17474	SPPRA ID WITHHELD	1575213087 Institute of Business Administration IBA Karachi Printing of Magazine		27 Sep 2013	27.Sep.2013	15.Oct.2013	BER & CS Required
17473	SPPRA ID WITHHELD	1575213086 Karachi Fisheries Harbor Authority KFHA Karachi Repair/Maintenance of Miscellaneous Work		27 Sep 2013	27.Sep.2013	23.Oct.2013	BER & CS Required
17472	SPPRA ID WITHHELD	1575213085 Executive Engineer Provincial Highway Division Mirpurkhas Construction of Roads		27 Sep 2013	26.Sep.2013	14.Oct.2013	BER & CS Required
17471	SPPRA ID WITHHELD	1575213084 Project Director Left Bank Outfall Drain LBOD Project Hyderabad Prequalification of Contractors/Firms		27 Sep 2013	27.Sep.2013	15.Oct.2013	BER & CS Required
17470	SPPRA ID WITHHELD	1575213083 Executive Engineer Provincial Coastal Highway Division Hyderabad Construction of Roads		27 Sep 2013	26.Sep.2013	11.Oct.2013	BER & CS Required
17469	SPPRA ID WITHHELD	1575213082 Executive Engineer Machinery Maintenance Division Digri @ Koldiji Construction of Roads		27 Sep 2013	26.Sep.2013	10.Oct.2013	BER & CS Required
17468	SPPRA ID WITHHELD	1575213081 Irrigation & Power Dept. Executive Engineer Irrigation West Division Khairpur		27 Sep 2013	26.Sep.2013	11.Oct.2013	BER & CS Required
17467	SPPRA ID WITHHELD	1575213080 Sindh Irrigation and Drainage Authority SIDA Hyderabad		27 Sep 2013	27.Sep.2013	15.Oct.2013	BER & CS Required
17466	SPPRA ID WITHHELD	1575213079 Irrigation & Power Dept. Executive Engineer Rohri Division Moro Construction of Roads		27 Sep 2013	26.Sep.2013	23.Oct.2013	BER & CS Required
1575213078		Sindh University					

ATTENDANCE SHEET

(Procurement Committee)

NAME OF WORK: SUPPLY & INSTALLATION OF ALUMINUM CLADDING / CURTAIN WALL, SINAGE / MURALS & INTERNAL EXTERNAL ALLIED DEVELOPMENT WORKS FOR THE PROJECT SHAHEED MOHTARMA BENAZIR BHUTTO ACCIDENT, EMERGENCY & TRAUMA CENTER AND ANCILLARY SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI

DATE OF OPENING: 08-10-2013 (TECHNICAL PROPOSALS)

S.NO.	MEMBERS	SIGNATURE	PHONE NUMBER
1.	Medical Superintendent Civil Hospital Karachi.		
2.	Chairperson, Department of Cardiology. Dow University of Health Sciences.		0300-2114853
3.	Chairperson, Department of Anaesthesia. Dow University of Health Sciences.		0300822004
4.	Chairman, Department of Neurosurgery. Dow University of Health Sciences.	for Prof. Inamd work 	03028722957
5.	Project Director		
6.	Addl. Director (Development), Health Department, Government of Sindh		
7.	Deputy Director (Development) Health Department, Government of Sindh		
8.	Divisional Accounts Officer A.G. Sindh Office		
9.	Accounts Officer Civil Hospital Karachi	 MUM 8/10/13	021-9925722 0332 3461459

10. CONSULTANT.
NABU & SON/DUIP/ASAC.



0308290105




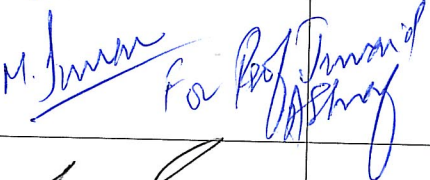








ATTENDANCE SHEET

(Procurement Committee)

NAME OF WORK: SUPPLY & INSTALLATION OF ALUMINUM CLADDING / CURTAIN WALL, SINAGE / MURALS & INTERNAL EXTERNAL ALLIED DEVELOPMENT WORKS FOR THE PROJECT SHAHEED MOHTARMA BENAZIR BHUTTO ACCIDENT, EMERGENCY & TRAUMA CENTER AND ANCILLARY SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI

DATE OF OPENING: 08-11-2013 (FINANCIAL PROPOSALS)

S.NO.	MEMBERS	SIGNATURE	PHONE NUMBER
1.	Medical Superintendent Civil Hospital Karachi.		
2.	Chairperson, Department of Cardiology. Dow University of Health Sciences.		
3.	Chairperson, Department of Anaesthesia. Dow University of Health Sciences.		03323102660
4.	Chairman, Department of Neurosurgery. Dow University of Health Sciences.		
5.	Project Director		
6.	Addl. Director (Development), Health Department, Government of Sindh		
7.	Deputy Director (Development) Health Department, Government of Sindh		
8.	Divisional Accounts Officer A.G. Sindh Office		
9.	Accounts Officer Civil Hospital Karachi		

10. A. BASHIR KHAN
MAJIN SIDDIQUE ASSE. 



Naqvi & Siddiquie Associates (PAKISTAN)
ARCHITECTS - ENGINEERS - PLANNERS - INTERIOR DESIGNERS - MANAGEMENT CONSULTANTS

NSA(P)-0223/2013/8806

28 OCT 2013

Project Director
Shaheed Mohtarma Benazir Bhutto Accident &
Emergency Centre and Allied Services Complex
Near O.P.D. Block, Civil Hospital
KARACHI.

**CONSTRUCTION OF SHAHEED MOHTARMA BENAZIR BHUTTO ACCIDENT & EMERGENCY
CENTRE AND ALLIED SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI**

EVALUATION REPORT OF TECHNICAL BIDS - PACKAGE-VII

(ALUMINUM CLADDING / CURTAIN WALL, SIGNAGE, MURALS & ALLIED WORKS)

Dear Sir

Technical & Financial Bids for Aluminum Cladding/Curtain Wall, Signage, Murals and allied works for the captioned project were invited through advertisement published in Daily Jang dated September 22, 2013 – In response following firms collected the documents and submitted their Bids on scheduled date ie 08-10-2013 :

- 1 M/s ALCOP
- 2 M/s Interact


Technical Bids opened in the presence of the Committee presided by Medical Superintendent, Civil Hospital Karachi which were forwarded to this office for scrutiny through letter bearing reference No. PD/ AEC & ASC /CHK/2013/2592 dated 08-10-2013 which we have checked and after scrutiny the status of marks obtained by both the firms are appended :

- 1). M/s ALCOP – **Recommended** for Prequalification as they have obtained 80% marks (more than fixed passing marks ie 75%)
- 2). M/s Interact - **Not recommended** for prequalification as they have obtained 45% marks (less than fixed passing marks ie 75%)

Technical Bids of both above Contracting Firms are attached along with Annexure-A (Evaluation Criteria showing the status of marks obtained by the firm) for your kind perusal, approval, record & further necessary action.

Thanking you and assuring you of our sincere cooperation at all time.

Yours sincerely
for Naqvi & Siddiquie Associates (Pakistan)


(Abdul Baseer Khan)
General Manager Engg. & Contracts

Encl: a. s. a.



NAQVI & SIDDIQUIE ASSOCIATES (Pakistan)

ANNEXURE - "A"

Shaheed Mohtarma Benazir Bhutto Accident, Emergency & Trauma Centre
And Ancillary Services Complex at Civil Hospital, Karachi.

SUMMARY OF EVALUATION CRITERIA FOR TECHNICAL PROPOSAL
For
(ALUMINIUM CLADDING / CURTAIN WALL, SIGNAGE, MURALS & ALLIED WORKS)

S. No.	NAME OF CONTRACTOR	Establishment /PEC Registration	Projects executed in last 5 years & in-hand			Valid Manufacturer's Authorization Certificate	T&P	List of Technical Staff	Financial stability	Last Three Years Tax Assessment	Affidavit / Certificate for no Blacklisting	Marks obtained	Remarks
			Above 20M (Aluminium Cladding)	Above 20M (Curtain Wall)	Above 10M (Signage)								
S. No. of Evaluation Criteria Break up of Marks		A	B	C	D	E	F	G	H	I	J		
		5	20	20	10	10	10	10	5	5	5	100	
1	M/S ALCOP	5	20	20	0	10	5	5	5	5	5	80	Since the contractor has supplied the required documents and obtained the marks which is above the passing marks hence this contractor is recommended for prequalification.
2	M/S INTERACT	5	5	5	0	5	5	5	5	5	5	45	Since the contractor has not provided the detail of project of required magnitude moreover not reached upto the passing marks hence he is not recommended for prequalification.


Total Marks : 100
Passing Marks : 75

Naqvi & Siddique Associates (Pakistan)
Karachi.


BID EVALUATION REPORT


1. Name of Procuring Agency: **Civil Hospital – Health Department**
 2. Tender Reference No: **PD-Trauma Centre-CHK/013 (Rev) (2013-14)**
 3. Tender Description / Name of Work/item: **“Supply & Installation of Aluminum Cladding / Curtain Wall, Sinage / Murals & Internal External Allied Development Works for the project “Shaheed Mohatarma Benazir Bhutto Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital Karachi”**
4. Method of Procurement: **Single Stage – Two Envelope**
 5. Tender Published: **Express – SPPRA Website**
 6. Total Bid documents Sold: **Two**
 7. Total Bids Received: **Two**
 8. Technical Bid Opening date: (if applicable) **08-10-2013**
 9. No. of Bid technically qualified (if applicable): **One**
 10. Bid(s) Rejected: **Nil**
 11. Financial Bid Opening date: **08-11-2013**
 12. **Bid Evaluation Report:**

S.No.	Name of Firm or Bidder	Cost offered by the Bidder	Ranking in terms of cost	Comparison with Estimated cost	Reasons for acceptances	Remarks
0	1	2	3	4	5	6
1.	M/S ALCOP	96,121,684/=	Lowest	Within overall cost of PC-I	On Lowest Basis	Recommended by Committee to award the work at a cost of Rs. 96,121,684/-.



Medical Superintendent
Civil Hospital Karachi



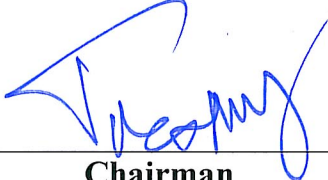Chairperson
Department of Cardiology


Chairperson
Department of Anaesthesia



Chairman
Department of Neurosurgery


Project Director


Director (Development),
Health Deptt: Govt. of Sindh


Deputy Director (Development),
Health Deptt: Govt. of Sindh


Divisional Accounts Officer
A.G. Sindh Office


Accounts Officer
Civil Hospital Karachi



**OFFICE OF THE PROJECT DIRECTOR
SHAHEED MOHTARMA BENAZIR BHUTTO
Accident, Emergency & Trauma Centre and Ancillary
Services Complex at Civil Hospital Karachi**

REPORT ON OPENING OF FINANCIAL PROPOSAL

SUBJECT: TENDER FOR THE WORK "SUPPLY & INSTALLATION OF ALUMINUM CLADDING / CURTAIN WALL, SINAGE / MURALS & INTERNAL EXTERNAL ALLIED DEVELOPMENT WORKS" FOR THE PROJECT "SHAHEED MOHTARMA BENAZAIR BHUTTO ACCIDENT, EMERGENCY & TRAUMA CENTER AND ANCILLARY SERVICES COMPLEX AT CIVIL HOSPITAL KARACHI"

- Financial Proposal of single technically qualified bidder was opened on 08-11-2013 at 11:00 a.m. before the following committee members:-
 1. Prof. M. Saeed Quraishy
Medical Superintendent – Civil Hospital Karachi / Chairman
 2. Prof. (Dr.) Khalida Soomro
Chairperson – Department of Cardiology, Dow University of Health Sciences / Member
 3. Prof. (Dr.) Sadqa Aftab
Chairperson – Department of Anaesthesia, Dow University of Health Sciences / Member
 4. Prof. (Dr.) Junaid Ashraf
Chairperson – Department of Neurosurgery, Dow University of Health Sciences / Member
 5. Engr. Hayat Kemal
Project Director / Member / Secretary
 6. Mrs. Shaista Mubarak
Additional Director (Development) Health Department – Govt. of Sindh / Member
 7. Dr. Abdul Jabbar Memon
Deputy Director (Development) Health Department – Govt. of Sindh / Member
 8. Mr. Saleem Ahmed Siddiqui
Divisional Accounts Officer – A.G. Sindh Office / Member
 9. Mr. Shahid Ali Khan
Accounts Officer – Civil Hospital Karachi / Member

- Following was the position after opening of Financial Bids:-

1) M/S ALCOP had quoted Rs. 96,121,684/=.

- Following is the Comparative Statement after the calculations arithmetically:-

S.No.	Contractors	Amount Quoted	Remarks / Result
1.	M/S ALCOP	Rs. 96,121,684/-	1 st Lowest

CONCLUSION

- In view of above M/S ALCOP are recommended to award of the work of **Supply & Installation of Aluminum Cladding / Curtain Wall, Sinage / Murals & Internal External Allied Development Works for the project "Shaheed Mohatarma Benazair Bhutto, Accident, Emergency & Trauma Centre and Ancillary Services Complex at Civil Hospital Karachi"** at the quoted cost of Rs. 96,121,684.00.


Medical Superintendent
Civil Hospital Karachi



Chairperson
Department of Cardiology


Chairperson
Department of Anaesthesia


Chairman
Department of Neurosurgery


Project Director


Director (Development),
Health Deptt: Govt. of Sindh


Deputy Director (Development),
Health Deptt: Govt. of Sindh


Divisional Accounts Officer
A.G. Sindh Office


Accounts Officer
Civil Hospital Karachi